

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027319.D
 Acq On : 12 Aug 2022 09:45
 Operator : SY/MD
 Sample : N4162-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC00

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027319.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	72	82	93	rBV	96580	111725	4.45%	1.322%
2	1.561	155	162	175	rVB	72761	79860	3.18%	0.945%
3	2.102	319	330	344	rBV	173111	248789	9.92%	2.943%
4	2.757	523	534	548	rBV2	26540	48930	1.95%	0.579%
5	3.185	653	667	682	rBV	12722	27297	1.09%	0.323%
6	3.902	874	890	923	rBV2	296289	835731	33.32%	9.886%
7	4.343	1010	1027	1054	rBV	121235	304822	12.15%	3.606%
8	4.603	1092	1108	1126	rBV3	45575	118833	4.74%	1.406%
9	5.044	1229	1245	1267	rBV3	259172	656229	26.17%	7.762%
10	5.613	1409	1422	1441	rBV	188915	395353	15.76%	4.676%
11	5.908	1500	1514	1529	rBV	1298100	2507990	100.00%	29.666%
12	5.973	1530	1534	1551	rVB3	50947	96032	3.83%	1.136%
13	6.066	1551	1563	1579	rBV	154951	314521	12.54%	3.720%
14	6.986	1839	1849	1868	rBV	59889	117239	4.67%	1.387%
15	7.314	1940	1951	1982	rBV	282589	528111	21.06%	6.247%
16	7.625	2037	2048	2059	rBV	35025	64716	2.58%	0.765%
17	8.088	2183	2192	2232	rBV	242628	515908	20.57%	6.102%
18	8.850	2418	2429	2448	rBV	304509	508498	20.28%	6.015%
19	10.214	2842	2853	2870	rBV	99732	161225	6.43%	1.907%
20	11.249	3164	3175	3198	rBV	264736	416676	16.61%	4.929%
21	11.622	3277	3291	3317	rBV	244835	395605	15.77%	4.679%




Sum of corrected areas: 8454090

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027319.D
Acq On : 12 Aug 2022 09:45
Operator : SY/MD
Sample : N4162-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

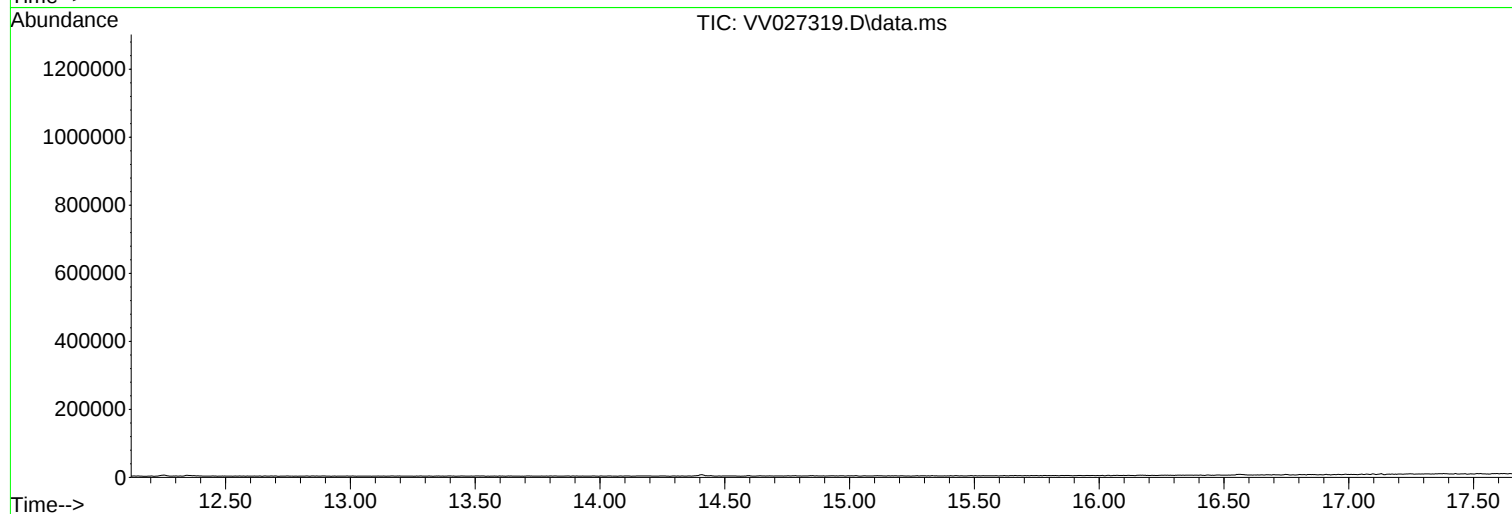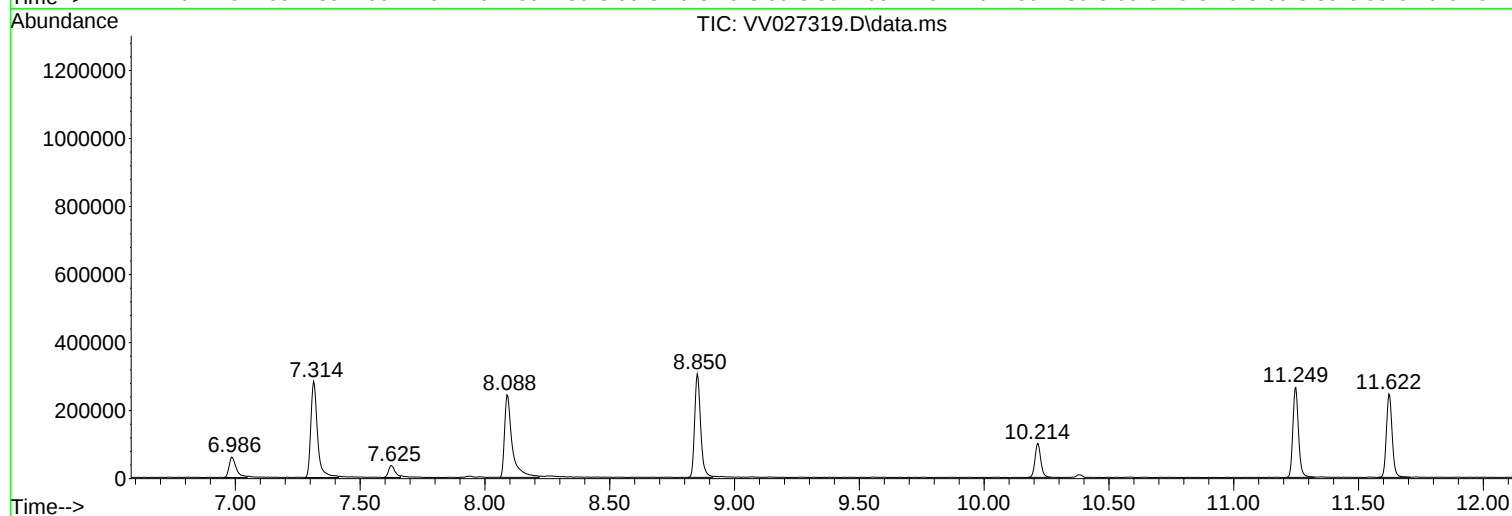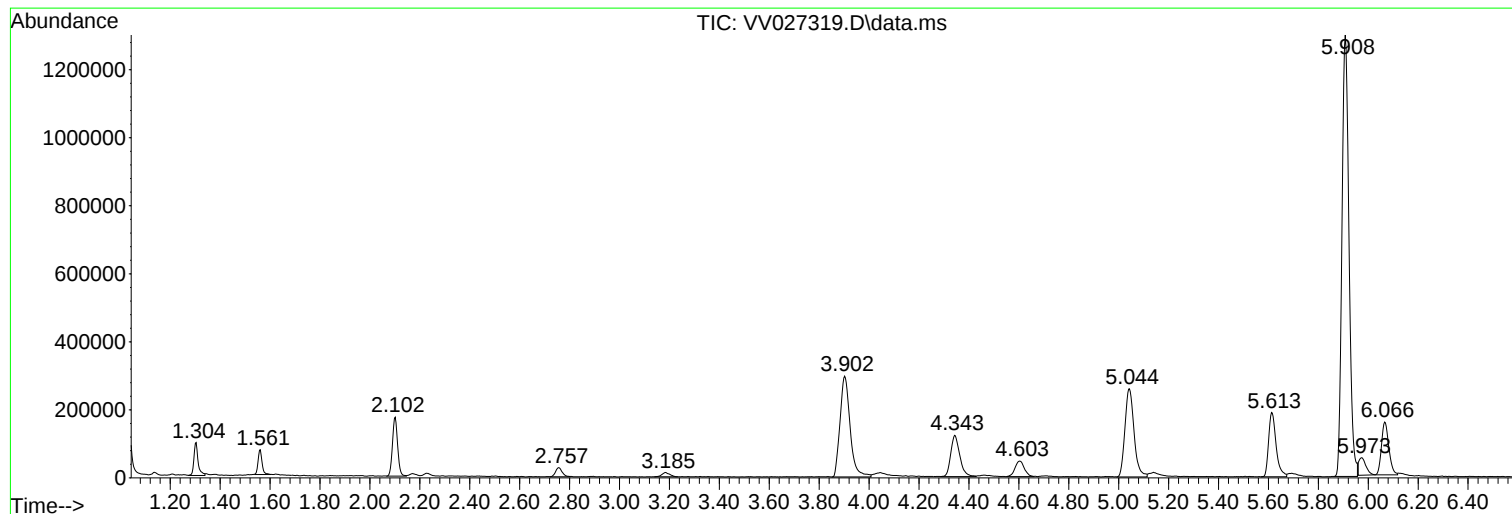

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027319.D
Acq On : 12 Aug 2022 09:45
Operator : SY/MD
Sample : N4162-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027319.D
Acq On : 12 Aug 2022 09:45
Operator : SY/MD
Sample : N4162-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc