

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027321.D
 Acq On : 12 Aug 2022 10:34
 Operator : SY/MD
 Sample : N4164-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC08

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.143	28	32	41	rVB	8828	9985	1.58%	0.204%
2	1.304	74	82	95	rBV	97355	106790	16.89%	2.182%
3	1.561	155	162	173	rBV	77308	84471	13.36%	1.726%
4	2.101	319	330	343	rBV	165506	237117	37.50%	4.844%
5	2.230	362	370	383	rVB4	8625	15859	2.51%	0.324%
6	3.886	876	885	906	rBV	47067	152752	24.16%	3.121%
7	4.342	1011	1027	1052	rBV2	113475	287341	45.44%	5.870%
8	5.043	1229	1245	1265	rBV2	256088	632350	100.00%	12.918%
9	5.140	1269	1275	1297	rVB4	10876	29964	4.74%	0.612%
10	5.613	1410	1422	1441	rBV	183333	384572	60.82%	7.856%
11	5.912	1503	1515	1527	rBV	4593	9803	1.55%	0.200%
12	6.066	1547	1563	1582	rBV	149041	319464	50.52%	6.526%
13	6.985	1838	1849	1868	rBV2	54132	111154	17.58%	2.271%
14	7.313	1939	1951	1980	rBV	266047	493647	78.07%	10.085%
15	7.625	2036	2048	2074	rBV2	32111	68346	10.81%	1.396%
16	8.092	2182	2193	2220	rBV	220895	498288	78.80%	10.180%
17	8.850	2417	2429	2456	rBV	293416	504238	79.74%	10.301%
18	10.217	2843	2854	2868	rBV2	95711	156266	24.71%	3.192%
19	10.384	2898	2906	2915	rVB2	6549	10051	1.59%	0.205%
20	11.249	3164	3175	3192	rBV	255741	404113	63.91%	8.256%
21	11.622	3280	3291	3312	rBV	236190	378431	59.85%	7.731%




Sum of corrected areas: 4895002

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027321.D
Acq On : 12 Aug 2022 10:34
Operator : SY/MD
Sample : N4164-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

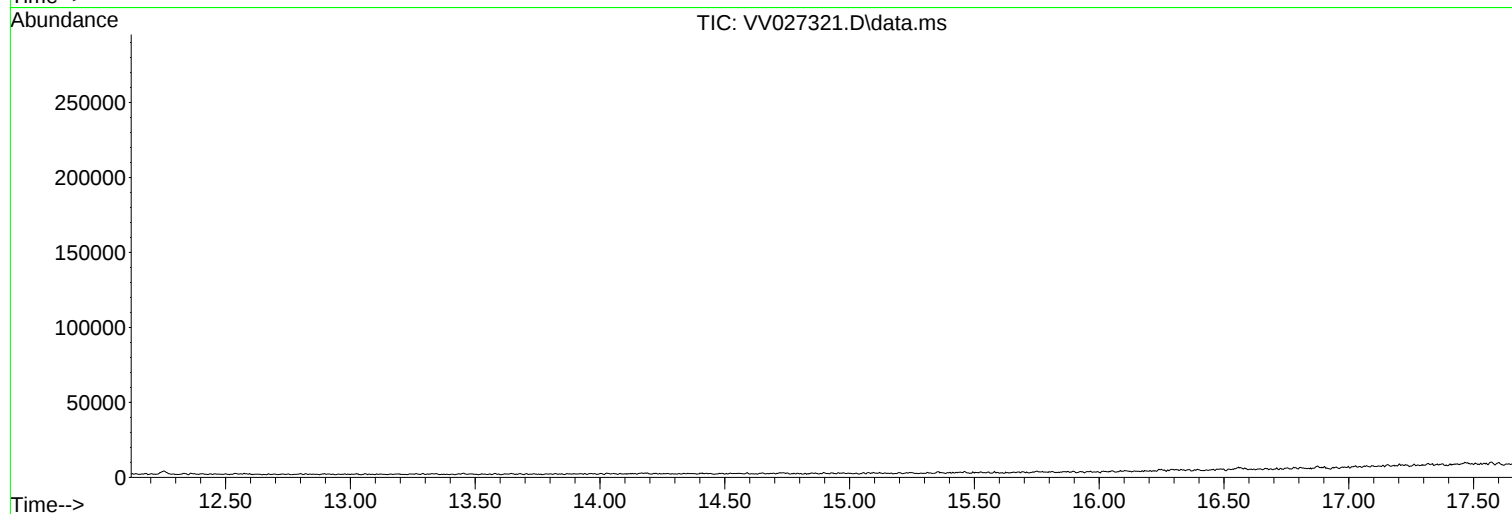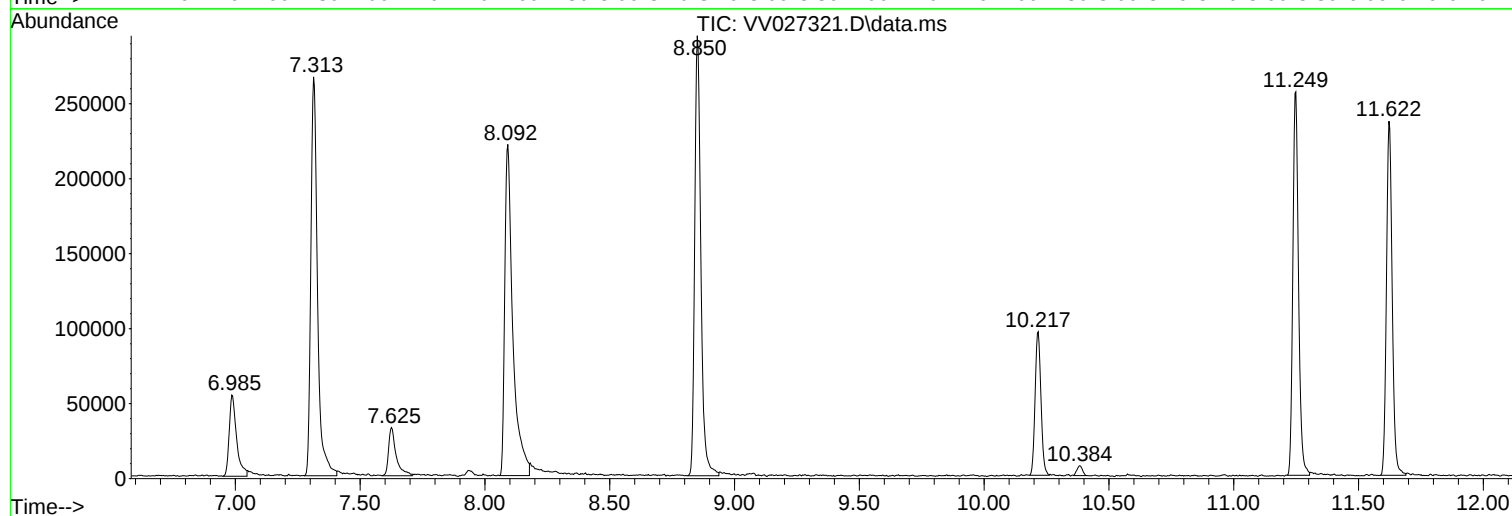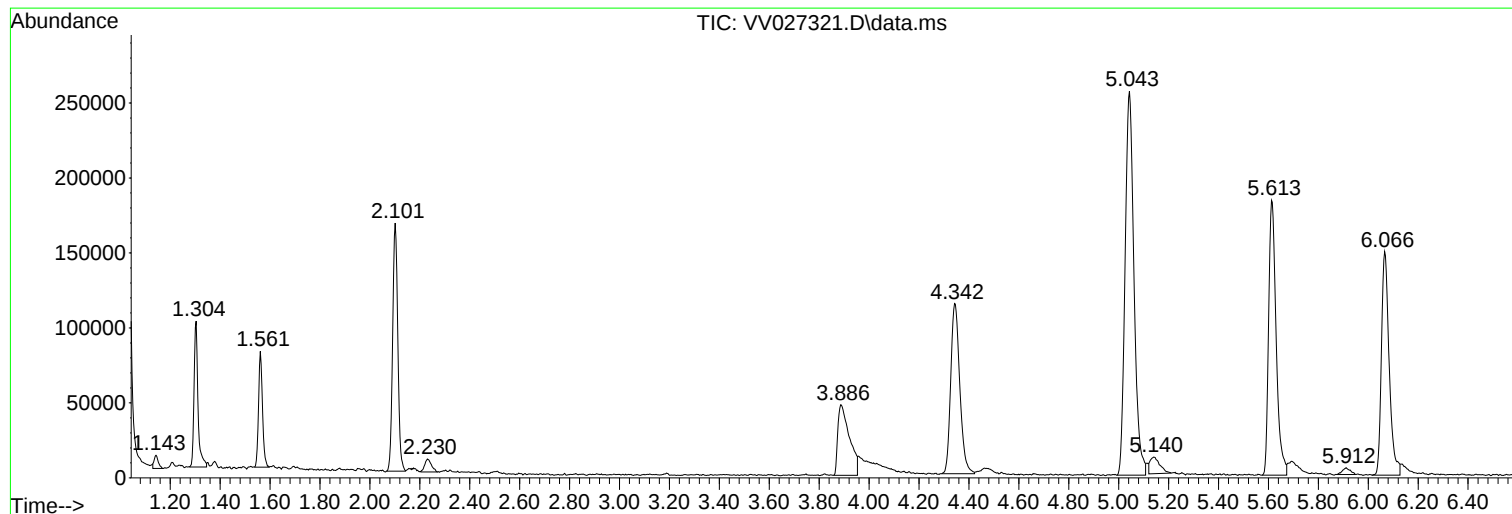

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027321.D
Acq On : 12 Aug 2022 10:34
Operator : SY/MD
Sample : N4164-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027321.D
Acq On : 12 Aug 2022 10:34
Operator : SY/MD
Sample : N4164-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc