

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027323.D
 Acq On : 12 Aug 2022 11:24
 Operator : SY/MD
 Sample : N4164-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027323.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.140	26	31	41	rVB	9011	12117	1.92%	0.241%
2	1.301	74	81	101	rVV	95910	106681	16.92%	2.122%
3	1.561	154	162	171	rBV	79605	88273	14.00%	1.756%
4	2.101	320	330	342	rVB	163716	230803	36.60%	4.591%
5	2.230	361	370	382	rVB3	9674	18551	2.94%	0.369%
6	3.889	876	886	923	rBV2	56774	199808	31.68%	3.974%
7	4.342	1011	1027	1053	rBV	115337	300190	47.60%	5.971%
8	5.043	1229	1245	1265	rBV2	250758	630640	100.00%	12.543%
9	5.146	1269	1277	1291	rVB4	10120	25458	4.04%	0.506%
10	5.613	1411	1422	1443	rBV	188702	395175	62.66%	7.860%
11	5.918	1502	1517	1534	rBV5	21883	52439	8.32%	1.043%
12	6.066	1550	1563	1580	rBV	148450	313064	49.64%	6.227%
13	6.985	1836	1849	1874	rBV	54009	113253	17.96%	2.253%
14	7.313	1940	1951	1971	rBV	269510	487646	77.33%	9.699%
15	7.622	2037	2047	2071	rBV	33389	65910	10.45%	1.311%
16	8.088	2182	2192	2236	rBV	231591	510669	80.98%	10.157%
17	8.850	2415	2429	2449	rBV	302177	514571	81.60%	10.235%
18	10.214	2841	2853	2871	rBV	95811	160041	25.38%	3.183%
19	10.384	2898	2906	2914	rVB4	4413	7079	1.12%	0.141%
20	11.249	3164	3175	3195	rBV	260513	415957	65.96%	8.273%
21	11.622	3280	3291	3309	rBV	235148	379482	60.17%	7.548%




Sum of corrected areas: 5027807

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027323.D
Acq On : 12 Aug 2022 11:24
Operator : SY/MD
Sample : N4164-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

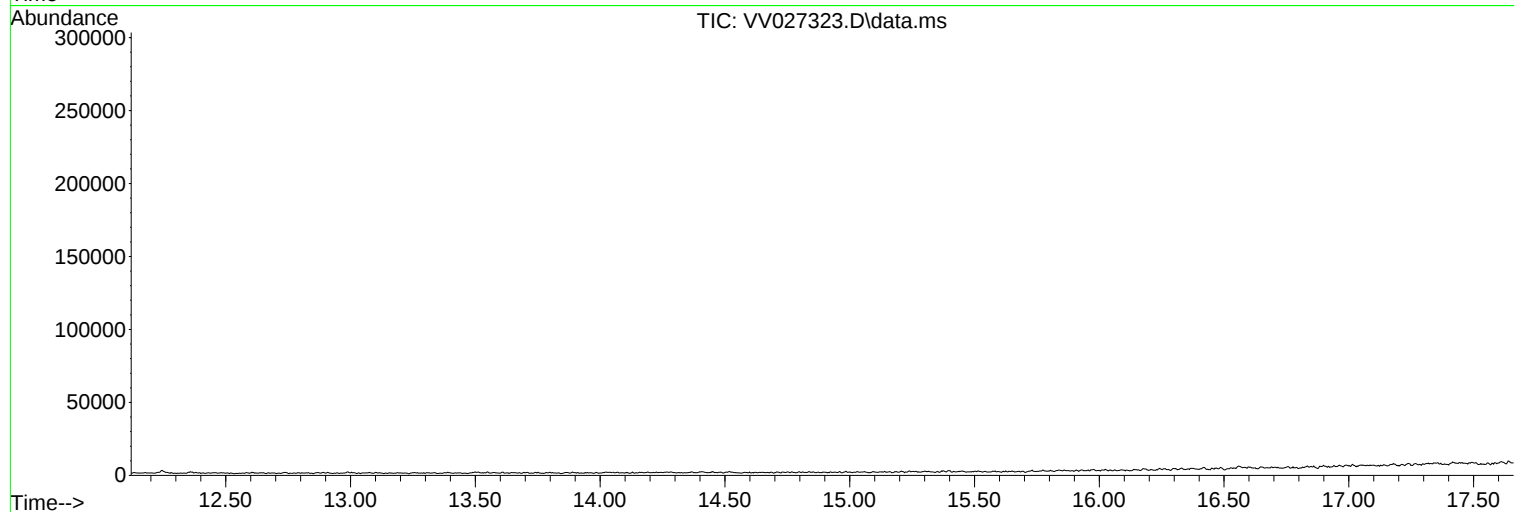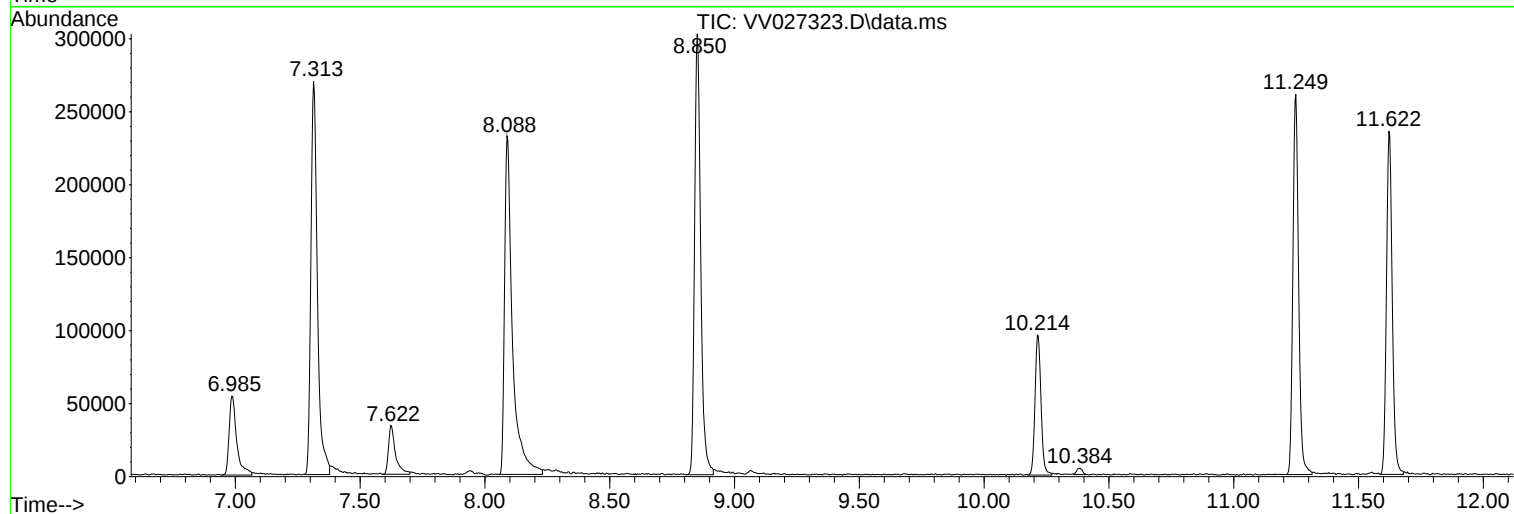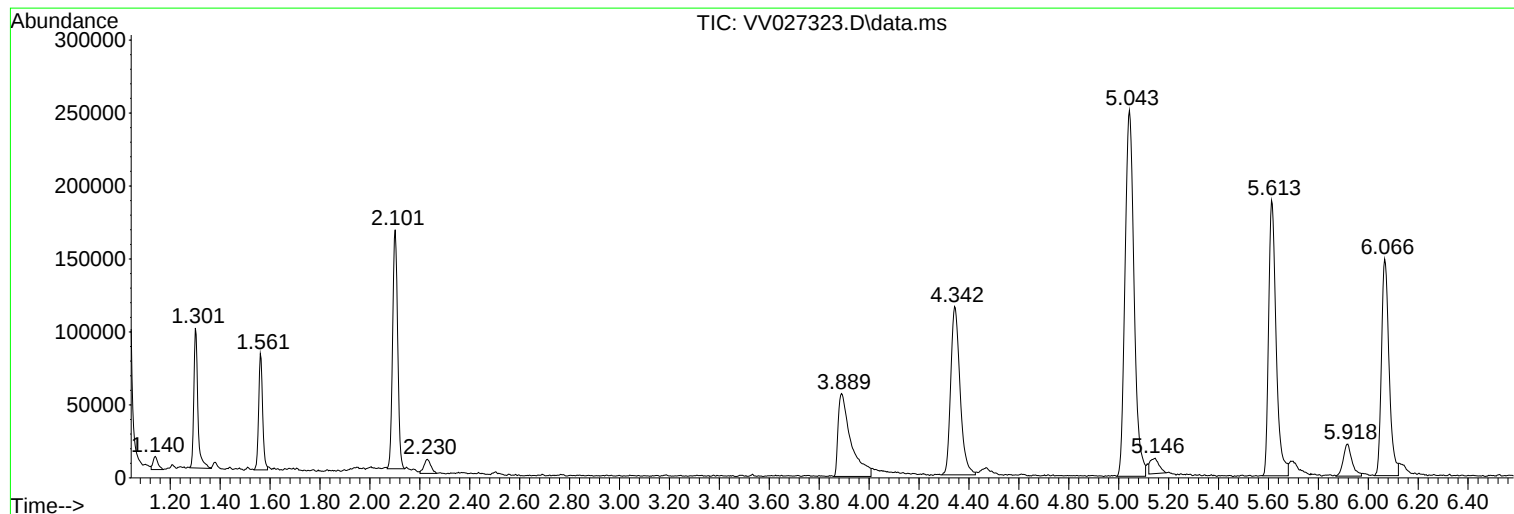

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027323.D
Acq On : 12 Aug 2022 11:24
Operator : SY/MD
Sample : N4164-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027323.D
Acq On : 12 Aug 2022 11:24
Operator : SY/MD
Sample : N4164-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc