

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027325.D
 Acq On : 12 Aug 2022 12:14
 Operator : SY/MD
 Sample : N4164-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC12

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027325.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.140	26	31	42	rVB	8433	11581	1.82%	0.230%
2	1.304	75	82	95	rBV	96299	106312	16.70%	2.113%
3	1.564	155	163	178	rVB	81799	93540	14.69%	1.859%
4	2.101	320	330	343	rBV	166692	234779	36.88%	4.666%
5	2.172	344	352	363	rVV	8166	16960	2.66%	0.337%
6	2.230	363	370	385	rVB2	11920	22108	3.47%	0.439%
7	3.892	877	887	910	rBV	48449	159704	25.08%	3.174%
8	4.346	1008	1028	1053	rBV	119938	305314	47.96%	6.068%
9	4.465	1055	1065	1074	rBV6	4561	9775	1.54%	0.194%
10	5.043	1227	1245	1264	rBV2	251379	636655	100.00%	12.654%
11	5.140	1267	1275	1293	rVB5	13721	37165	5.84%	0.739%
12	5.616	1410	1423	1441	rBV2	176900	366566	57.58%	7.286%
13	6.069	1550	1564	1580	rBV	149722	318568	50.04%	6.332%
14	6.989	1837	1850	1876	rBV2	54526	114775	18.03%	2.281%
15	7.313	1940	1951	1974	rBV	271203	505952	79.47%	10.056%
16	7.625	2038	2048	2062	rBV	32459	63481	9.97%	1.262%
17	8.091	2183	2193	2226	rBV	226565	532234	83.60%	10.579%
18	8.252	2239	2243	2254	rVB9	3846	6536	1.03%	0.130%
19	8.850	2418	2429	2455	rBV	288195	499417	78.44%	9.926%
20	10.217	2844	2854	2869	rVB	99308	161114	25.31%	3.202%
21	10.384	2896	2906	2912	rBV8	4854	7048	1.11%	0.140%
22	11.249	3162	3175	3194	rBV	252940	398360	62.57%	7.918%
23	11.352	3198	3207	3218	rVB10	6258	9389	1.47%	0.187%
24	11.622	3280	3291	3314	rBV	242321	391364	61.47%	7.779%
25	12.348	3506	3517	3528	rBV7	8429	14053	2.21%	0.279%
26	14.406	4148	4157	4165	rBV10	5178	8500	1.34%	0.169%




Sum of corrected areas: 5031250

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027325.D
Acq On : 12 Aug 2022 12:14
Operator : SY/MD
Sample : N4164-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

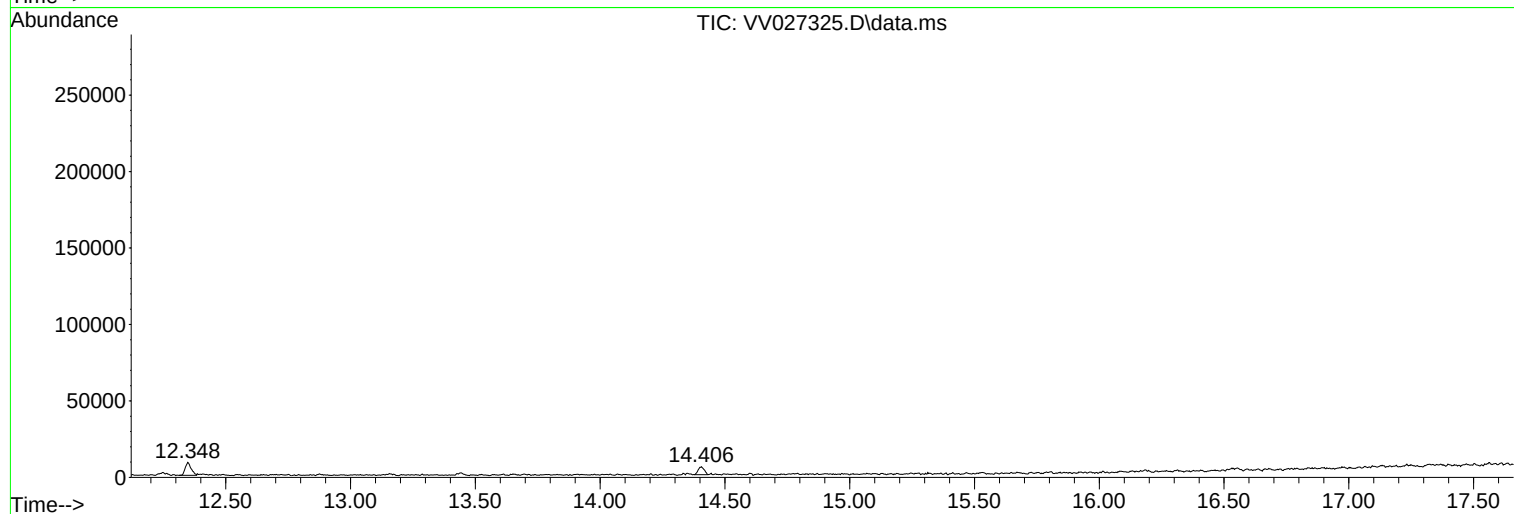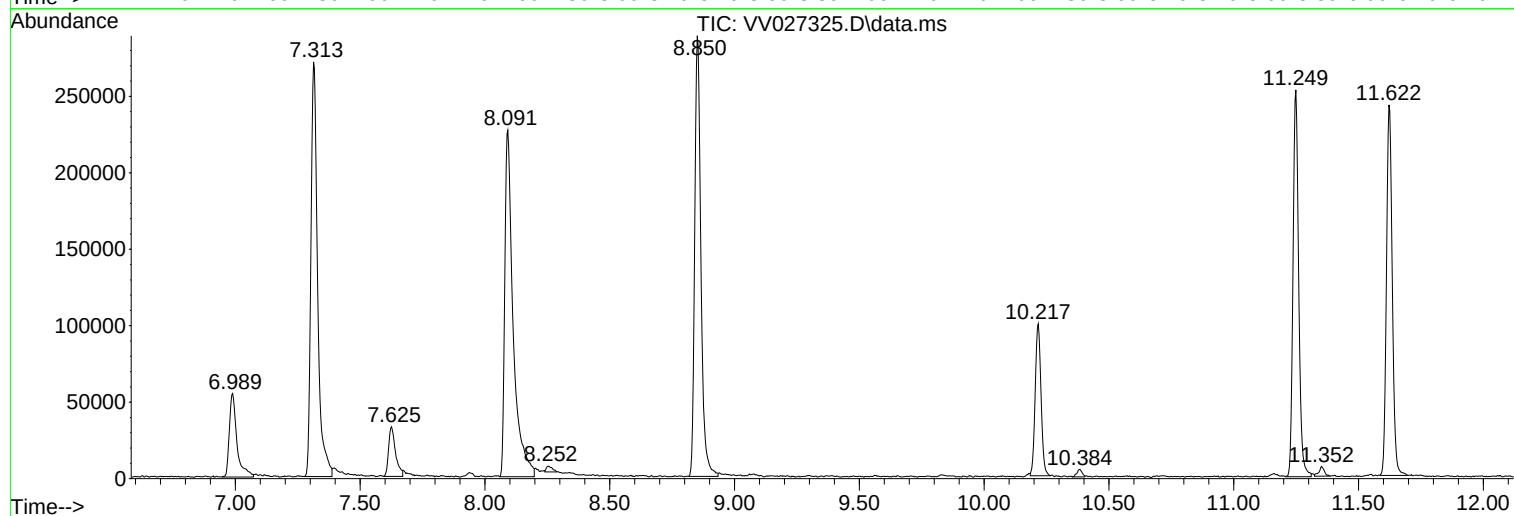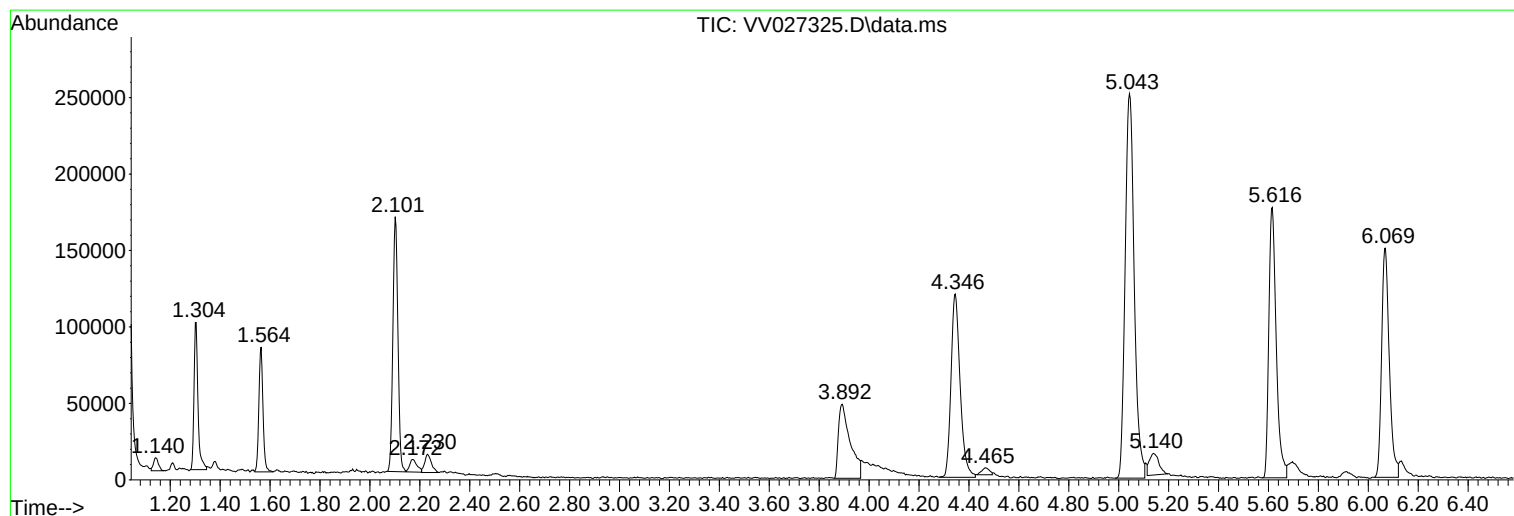

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027325.D
Acq On : 12 Aug 2022 12:14
Operator : SY/MD
Sample : N4164-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027325.D
Acq On : 12 Aug 2022 12:14
Operator : SY/MD
Sample : N4164-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
