

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027329.D
 Acq On : 12 Aug 2022 13:54
 Operator : SY/MD
 Sample : N4145-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY148

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027329.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	57	62	74	rVV7	3623	6773	1.18%	0.137%
2	1.304	74	82	102	rVV	83924	95996	16.69%	1.936%
3	1.561	154	162	174	rVB	66566	75508	13.13%	1.523%
4	2.101	320	330	345	rVV	144330	207391	36.07%	4.183%
5	2.169	345	351	362	rVB8	3673	6487	1.13%	0.131%
6	2.243	365	374	384	rBV2	9206	15514	2.70%	0.313%
7	2.503	446	455	464	rBV8	3854	6286	1.09%	0.127%
8	3.883	875	884	920	rBV	68355	207484	36.08%	4.185%
9	4.346	1011	1028	1052	rBV2	108781	276558	48.09%	5.578%
10	4.471	1056	1067	1081	rVB6	4555	11547	2.01%	0.233%
11	5.043	1228	1245	1267	rBV3	228250	575034	100.00%	11.599%
12	5.150	1269	1278	1295	rVB3	10858	27654	4.81%	0.558%
13	5.613	1409	1422	1441	rBV	198096	412260	71.69%	8.315%
14	5.699	1444	1449	1465	rVB	9522	22640	3.94%	0.457%
15	5.905	1505	1513	1519	rBV8	4764	8131	1.41%	0.164%
16	6.069	1549	1564	1580	rBV	141165	294775	51.26%	5.946%
17	6.985	1838	1849	1864	rBV2	55468	109028	18.96%	2.199%
18	7.313	1937	1951	1974	rBV	237997	443346	77.10%	8.943%
19	7.625	2038	2048	2061	rBV	34826	65461	11.38%	1.320%
20	7.789	2087	2099	2116	rBV3	20721	39742	6.91%	0.802%
21	8.088	2182	2192	2227	rBV	242144	525229	91.34%	10.594%
22	8.850	2417	2429	2450	rBV	321127	540869	94.06%	10.910%
23	10.217	2840	2854	2868	rBV	94383	155314	27.01%	3.133%
24	10.378	2895	2904	2912	rBV7	4339	7935	1.38%	0.160%
25	11.249	3163	3175	3196	rBV	277605	439942	76.51%	8.874%
26	11.538	3254	3265	3277	rBV3	9036	18814	3.27%	0.379%
27	11.622	3280	3291	3312	rVB	226235	362014	62.96%	7.302%




Sum of corrected areas: 4957732

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027329.D
Acq On : 12 Aug 2022 13:54
Operator : SY/MD
Sample : N4145-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY148

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

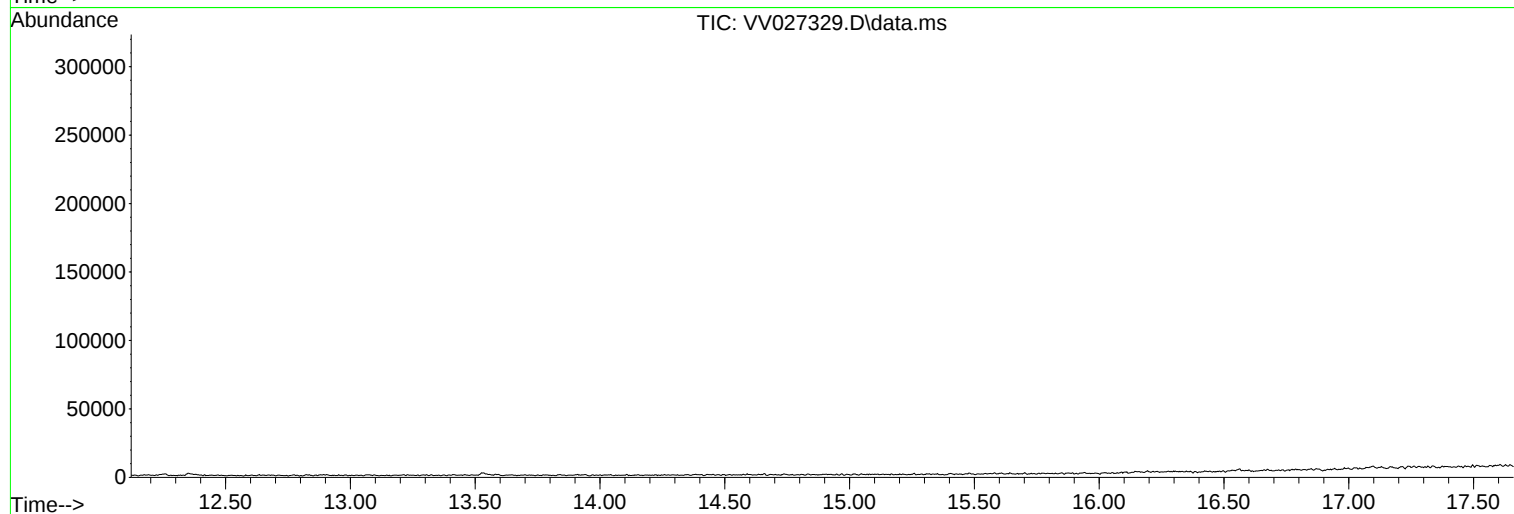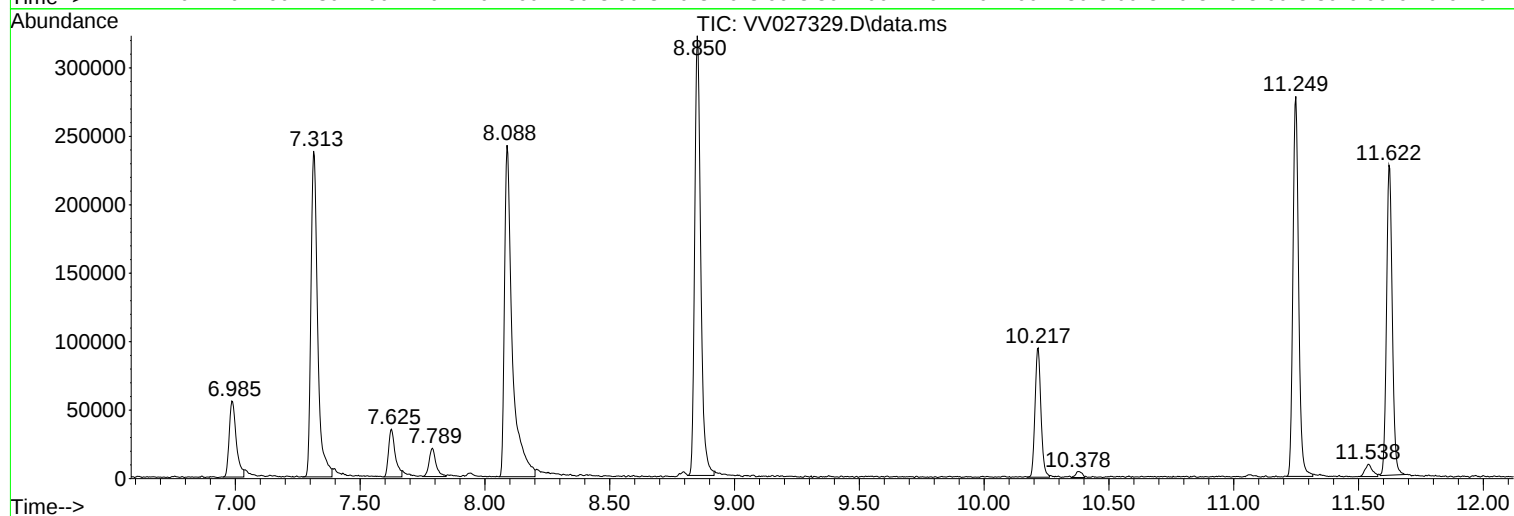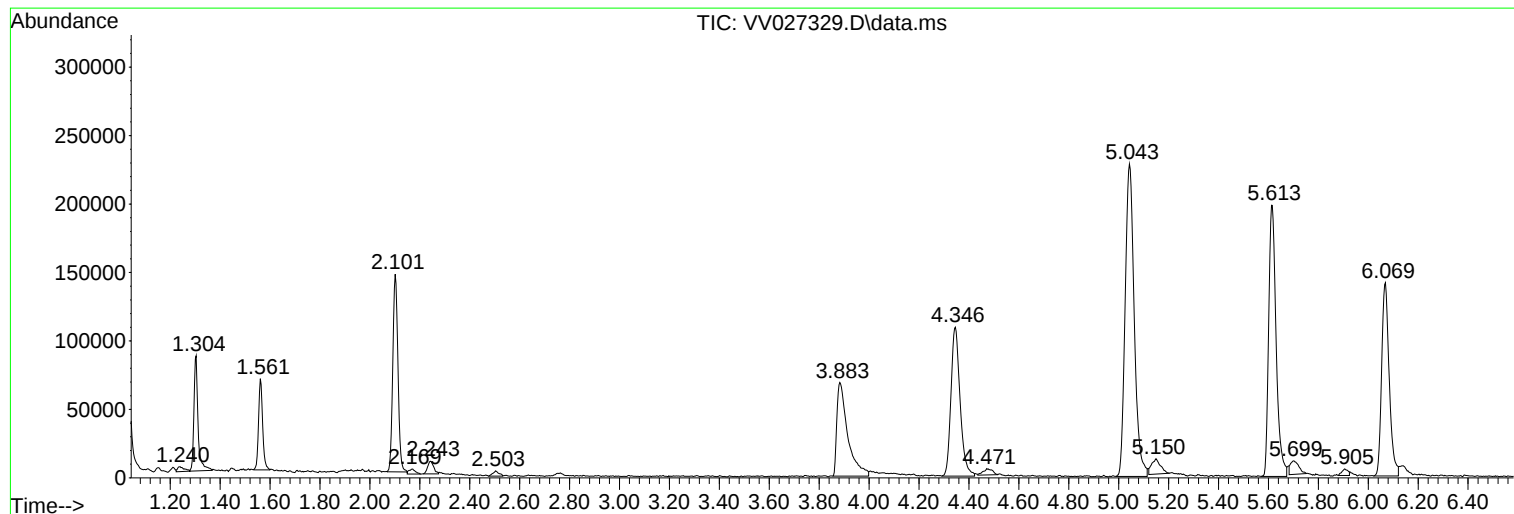

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027329.D
Acq On : 12 Aug 2022 13:54
Operator : SY/MD
Sample : N4145-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY148

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027329.D
Acq On : 12 Aug 2022 13:54
Operator : SY/MD
Sample : N4145-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY148

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc