

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027336.D
 Acq On : 12 Aug 2022 18:45
 Operator : SY/MD
 Sample : VV0812WBL03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK202

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027336.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	39	45	50	rBV	8827	9412	1.43%	0.172%
2	1.301	73	81	93	rBV	92306	99172	15.06%	1.808%
3	1.561	155	162	178	rVB	74728	85536	12.99%	1.559%
4	2.101	318	330	346	rBV	158803	230154	34.96%	4.195%
5	2.275	374	384	402	rVB3	12760	27011	4.10%	0.492%
6	2.500	444	454	469	rBV	19315	32265	4.90%	0.588%
7	3.889	874	886	914	rBV3	64688	256295	38.93%	4.672%
8	4.343	1010	1027	1053	rBV	116668	295052	44.82%	5.378%
9	4.497	1061	1075	1087	rBV3	6939	17550	2.67%	0.320%
10	5.040	1227	1244	1265	rBV2	265101	658375	100.00%	12.001%
11	5.162	1274	1282	1303	rVB4	13883	35496	5.39%	0.647%
12	5.613	1406	1422	1444	rBV	201460	426117	64.72%	7.767%
13	5.712	1445	1453	1467	rVB3	9760	21638	3.29%	0.394%
14	5.908	1503	1514	1522	rBV10	4760	9521	1.45%	0.174%
15	6.066	1547	1563	1581	rBV	152953	321482	48.83%	5.860%
16	6.143	1584	1587	1601	rVB6	7602	14122	2.14%	0.257%
17	6.982	1839	1848	1866	rBV	67694	133388	20.26%	2.431%
18	7.314	1937	1951	1978	rBV	290244	545599	82.87%	9.945%
19	7.622	2038	2047	2067	rBV	39897	78197	11.88%	1.425%
20	8.088	2181	2192	2222	rBV	234118	533266	81.00%	9.720%
21	8.420	2286	2295	2307	rBV4	10447	21716	3.30%	0.396%
22	8.850	2418	2429	2451	rBV	319462	548250	83.27%	9.993%
23	10.214	2841	2853	2867	rBV	100531	165172	25.09%	3.011%
24	11.249	3162	3175	3199	rBV	289719	459116	69.73%	8.369%
25	11.622	3280	3291	3311	rBV	264833	426846	64.83%	7.780%
26	13.265	3792	3802	3812	rVB6	4894	8265	1.26%	0.151%
27	13.509	3870	3878	3891	rBV	10097	17145	2.60%	0.313%
28	13.747	3944	3952	3963	rBV9	6143	9978	1.52%	0.182%




Sum of corrected areas: 5486136

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027336.D
Acq On : 12 Aug 2022 18:45
Operator : SY/MD
Sample : VV0812WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

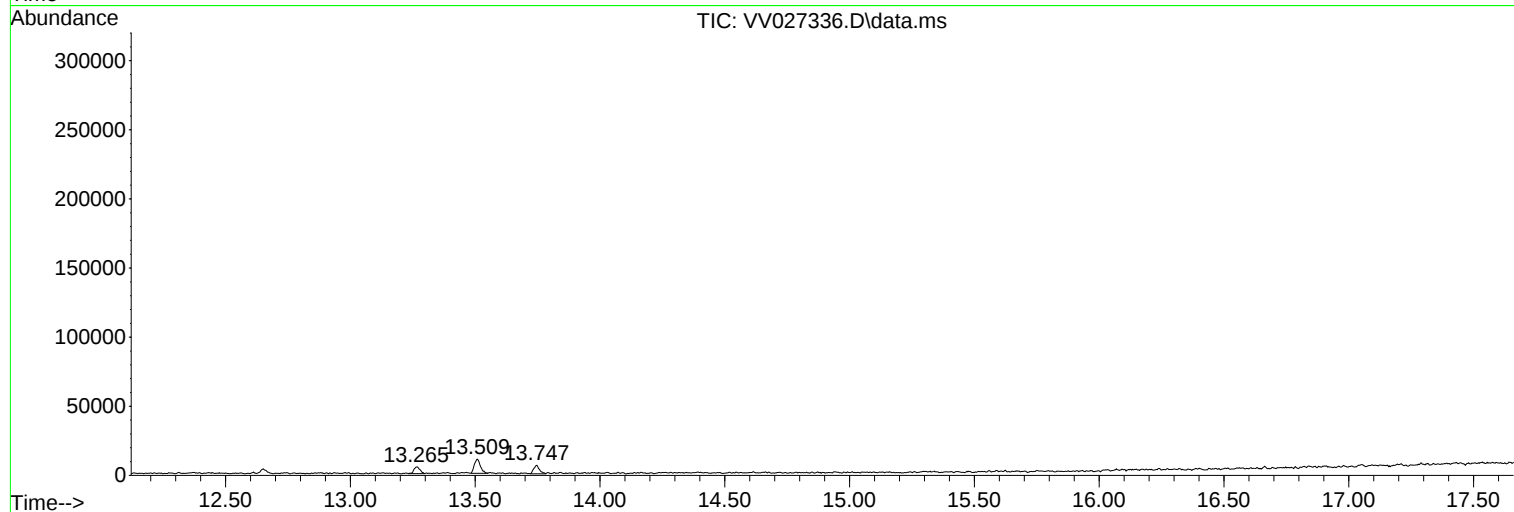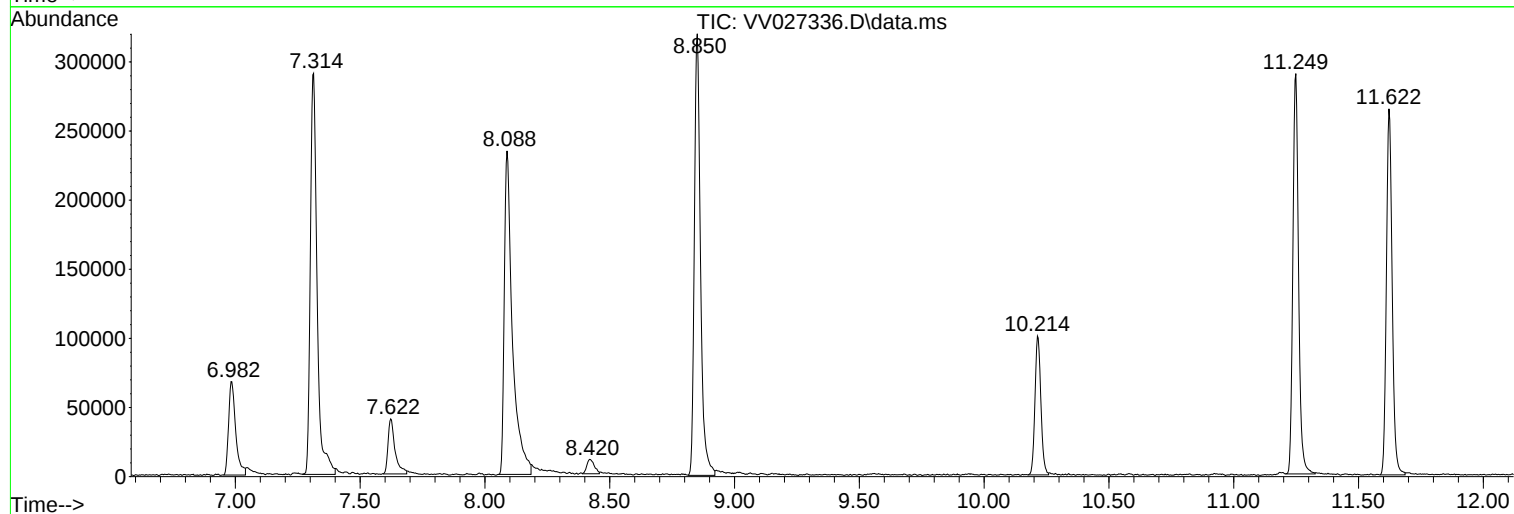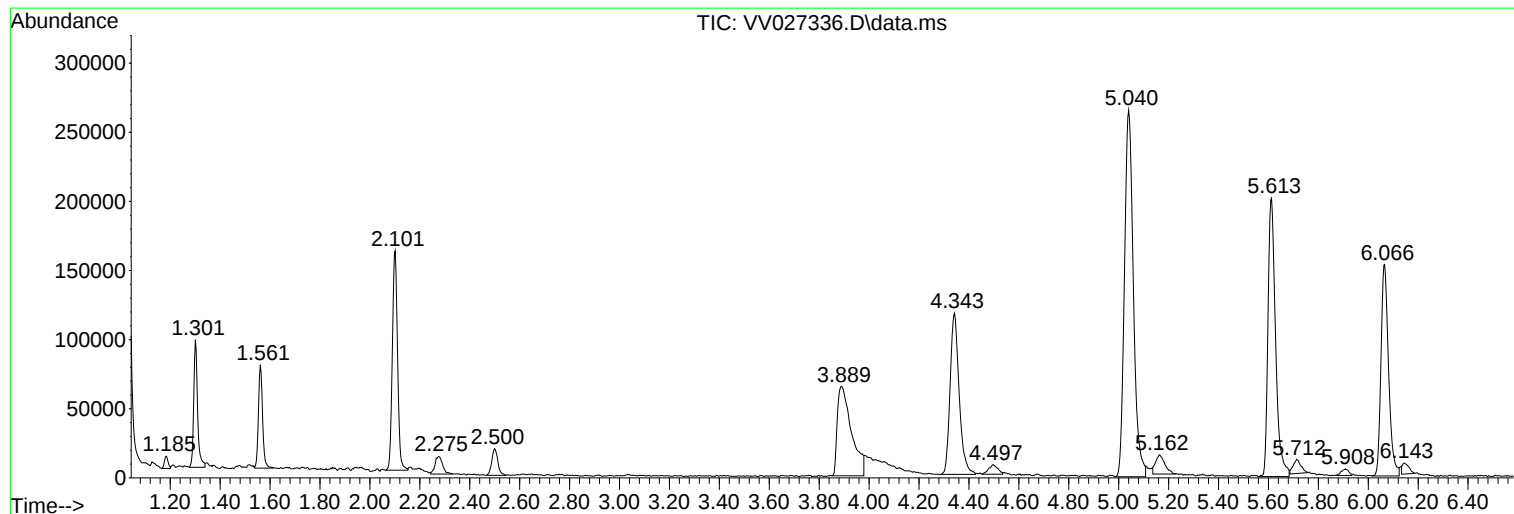

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027336.D
Acq On : 12 Aug 2022 18:45
Operator : SY/MD
Sample : VV0812WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027336.D
Acq On : 12 Aug 2022 18:45
Operator : SY/MD
Sample : VV0812WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc