


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027284.D
Acq On : 11 Aug 2022 16:32
Operator : SY/MD
Sample : BFB351
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB351

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Aug 13 21:49:38 2022

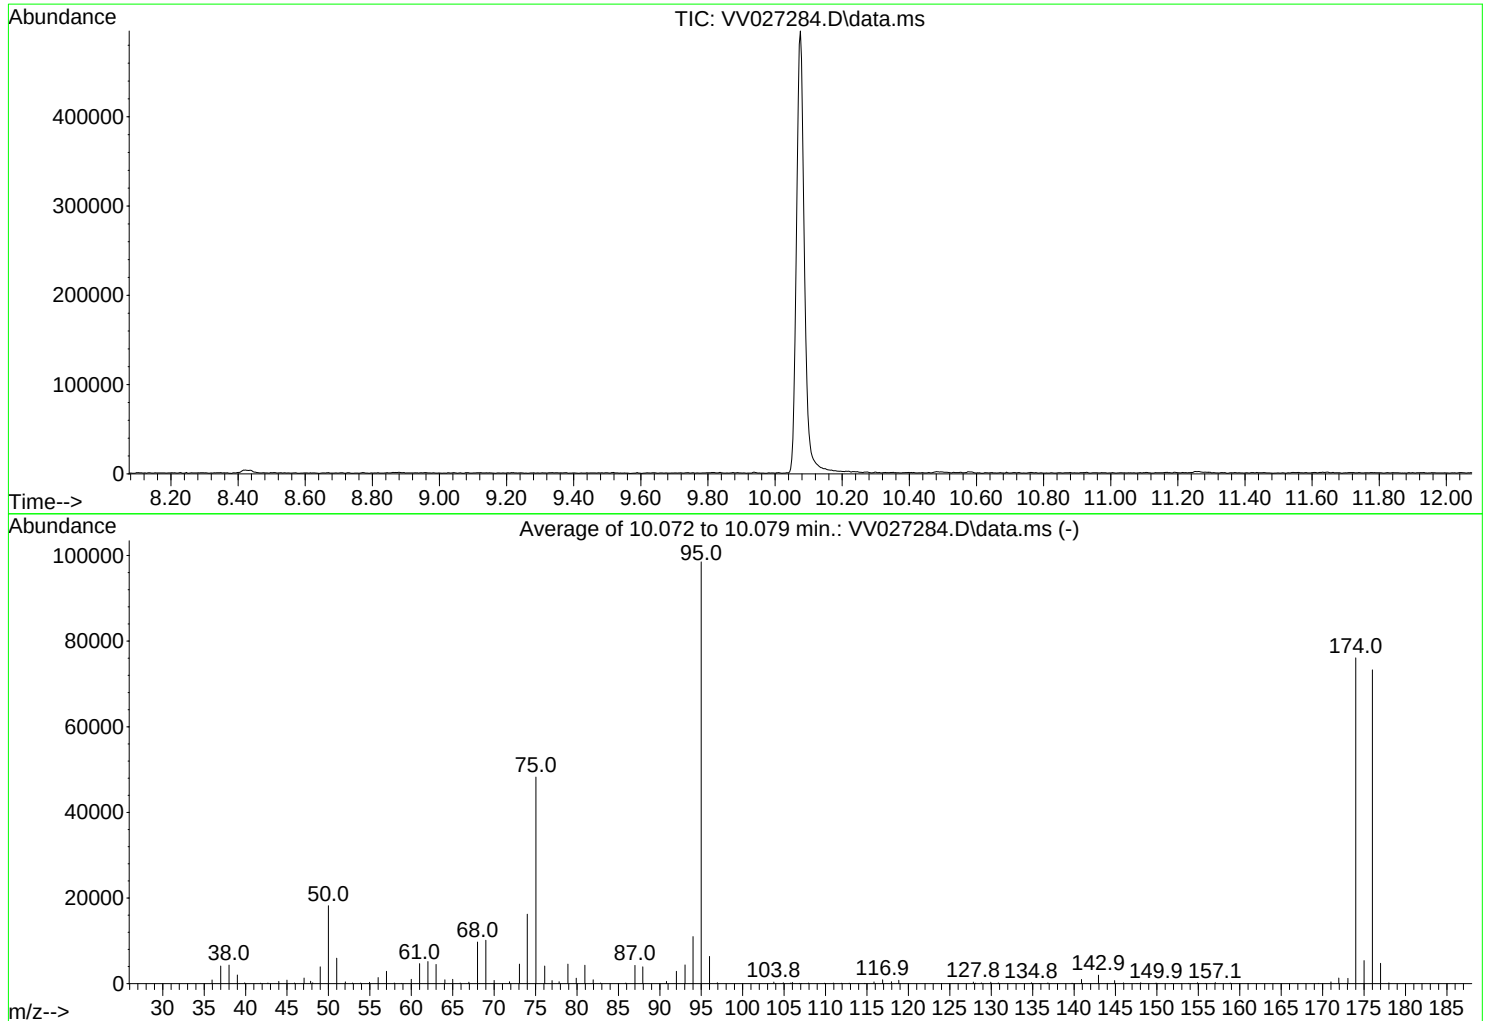

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	18203	PASS
75	95	30	80	49.0	48261	PASS
95	95	100	100	100.0	98523	PASS
96	95	5	9	6.4	6339	PASS
173	174	0.00	2	1.6	1240	PASS
174	95	50	120	77.2	76109	PASS
175	174	5	9	7.1	5391	PASS
176	174	95	105	96.3	73280	PASS
177	176	5	10	6.5	4736	PASS

m/z	Abundance
36.00	123.0
38.00	102.0
39.90	248.0
44.00	411.0
50.50	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351

m/z	Abundance
36.00	910.0
37.00	4133.0
38.00	4487.0
39.00	1959.0
39.90	405.0
41.80	132.0
42.70	109.0
44.00	966.0
45.00	868.0
45.90	217.0
47.00	1337.0
47.90	643.0
49.00	3982.0
50.00	18360.0
51.00	6070.0
52.10	400.0
53.00	163.0
53.90	116.0
55.00	320.0
56.00	1484.0
57.00	2980.0
57.90	132.0
58.80	118.0
60.00	983.0
61.00	4982.0
62.00	5309.0
63.00	4432.0
64.10	990.0
65.00	1002.0
65.90	180.0
67.00	336.0
68.00	9891.0
69.00	10258.0
70.00	698.0
71.90	547.0
73.00	4734.0
74.00	16180.0
75.00	48832.0
76.10	4268.0
76.90	730.0
77.90	359.0
78.90	4457.0
79.90	1318.0
80.90	4406.0
81.90	912.0
82.90	113.0
85.90	179.0
87.00	4371.0
87.90	3940.0
90.80	509.0
92.00	2961.0
93.00	4341.0
94.00	11149.0
95.00	99056.0
96.00	6566.0
96.90	244.0
103.70	393.0
104.90	224.0
105.80	452.0
106.80	153.0
107.90	122.0
109.90	112.0
111.00	160.0
111.90	110.0
113.00	112.0
115.80	504.0
116.90	826.0
117.90	411.0
118.80	768.0
124.00	102.0
127.80	399.0
128.80	152.0
129.90	353.0
130.90	162.0
134.90	213.0
136.90	194.0
139.80	106.0
140.90	971.0
142.90	1933.0
144.00	135.0
144.90	721.0
146.00	191.0
147.60	141.0
148.10	174.0
149.90	164.0
152.90	118.0
153.80	126.0
154.90	230.0
157.10	276.0
158.90	171.0
161.00	102.0
169.50	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351

171.00	380.0
171.90	1369.0
173.10	1327.0
174.00	75128.0
175.00	5410.0
176.00	71688.0
177.00	4622.0
178.00	170.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351

m/z	Abundance
35.90	1008.0
37.00	4203.0
38.00	4624.0
39.00	2038.0
39.90	454.0
41.80	128.0
42.70	139.0
44.00	946.0
45.00	864.0
45.90	157.0
47.10	1350.0
47.90	596.0
49.00	4041.0
50.00	18856.0
51.00	6168.0
52.10	414.0
52.90	157.0
53.90	139.0
55.00	327.0
56.00	1377.0
57.00	2957.0
57.90	145.0
58.80	107.0
60.00	1037.0
61.00	4790.0
62.00	5341.0
63.00	4656.0
64.10	910.0
65.00	1066.0
65.90	159.0
67.00	337.0
68.00	10034.0
69.00	10425.0
70.00	754.0
71.90	487.0
73.00	4736.0
74.00	16656.0
75.10	49920.0
76.10	4240.0
77.00	725.0
77.90	510.0
78.90	4686.0
79.90	1311.0
81.00	4448.0
82.00	896.0
82.80	166.0
85.90	138.0
87.00	4406.0
87.90	4067.0
90.80	545.0
92.00	2977.0
93.10	4499.0
94.00	11204.0
95.00	102192.0
96.00	6553.0
97.00	240.0
103.80	391.0
104.90	224.0
106.00	448.0
106.90	120.0
108.00	149.0
109.90	126.0
110.90	139.0
111.90	117.0
112.80	118.0
114.80	101.0
115.80	440.0
116.90	923.0
118.00	474.0
118.90	778.0
127.90	417.0
128.80	177.0
129.90	331.0
130.80	190.0
134.80	211.0
135.80	124.0
136.80	184.0
139.70	136.0
140.90	974.0
142.90	2011.0
144.00	113.0
144.90	725.0
146.00	189.0
148.10	213.0
149.90	143.0
153.80	107.0
154.90	248.0
155.90	122.0
157.10	271.0
158.90	171.0
169.50	125.0
171.00	402.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351

171.90	1330.0
173.00	1285.0
174.00	78672.0
175.00	5541.0
176.00	75672.0
177.00	4889.0
178.00	191.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351

m/z	Abundance
35.90	985.0
37.00	4011.0
38.00	4236.0
39.00	2029.0
39.90	449.0
41.80	113.0
42.70	169.0
44.00	937.0
45.00	757.0
45.90	128.0
47.10	1188.0
47.80	500.0
48.10	531.0
49.00	3755.0
50.00	17392.0
51.00	5553.0
52.00	394.0
52.80	158.0
53.90	166.0
54.90	307.0
56.00	1409.0
57.00	2682.0
58.00	142.0
60.00	1003.0
61.00	4272.0
62.00	4885.0
63.00	4382.0
64.00	789.0
65.00	981.0
65.90	136.0
66.90	306.0
68.00	9192.0
69.00	9673.0
70.00	771.0
71.80	377.0
73.10	4213.0
74.00	15813.0
75.00	46032.0
76.10	3824.0
77.10	671.0
77.80	538.0
78.90	4492.0
79.90	1175.0
80.90	4021.0
81.90	848.0
82.80	176.0
85.90	140.0
87.00	4068.0
88.00	3763.0
90.80	482.0
92.00	2721.0
93.10	4246.0
94.00	10631.0
95.00	94320.0
96.00	5897.0
97.00	217.0
103.80	376.0
104.90	187.0
106.00	418.0
107.10	103.0
108.00	151.0
109.90	128.0
110.90	114.0
111.90	150.0
112.70	127.0
114.70	124.0
115.90	333.0
116.90	931.0
117.90	460.0
118.90	766.0
127.90	339.0
128.10	344.0
128.80	212.0
130.00	303.0
130.80	212.0
134.80	205.0
136.80	170.0
139.70	135.0
140.90	927.0
143.00	1948.0
144.90	729.0
145.80	190.0
148.00	244.0
149.90	101.0
151.80	101.0
154.90	254.0
155.90	129.0
157.00	225.0
158.80	135.0
171.00	435.0
172.00	1252.0
173.00	1107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351

174.00	74528.0
175.00	5223.0
176.00	72480.0
177.00	4697.0
178.00	195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351