

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081224\
 Data File : VV036901.D
 Acq On : 12 Aug 2024 13:29
 Operator : SY/MD
 Sample : P3533-11
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	402480	428237	15.05%	2.103%
2	1.532	146	153	169	rVB	324492	382864	13.45%	1.880%
3	2.060	308	317	329	rBV	662318	948628	33.33%	4.659%
4	3.796	849	857	885	rBV	145020	392937	13.81%	1.930%
5	4.246	982	997	1025	rBV	436121	1103934	38.79%	5.422%
6	4.748	1150	1153	1155	rBV3	1847	937	0.03%	0.005%
7	4.764	1155	1158	1162	rVV6	1433	784	0.03%	0.004%
8	4.873	1189	1192	1193	rBV3	554	320	0.01%	0.002%
9	4.950	1200	1216	1245	rBV2	1139242	2846279	100.00%	13.979%
10	5.529	1385	1396	1427	rBV	793775	1633090	57.38%	8.021%
11	5.825	1477	1488	1507	rBV3	50046	116707	4.10%	0.573%
12	5.985	1526	1538	1561	rBV	618769	1270663	44.64%	6.241%
13	6.477	1690	1691	1695	rBV4	1133	766	0.03%	0.004%
14	6.625	1735	1737	1740	rVB4	839	429	0.02%	0.002%
15	6.641	1740	1742	1744	rBV3	904	292	0.01%	0.001%
16	6.661	1746	1748	1750	rVV3	1044	396	0.01%	0.002%
17	6.802	1789	1792	1795	rVB4	1993	1248	0.04%	0.006%
18	6.818	1795	1797	1799	rBV3	848	467	0.02%	0.002%
19	6.857	1806	1809	1812	rVB4	1938	1165	0.04%	0.006%
20	6.911	1812	1826	1850	rBV	350395	666760	23.43%	3.275%
21	7.239	1916	1928	1950	rBV	1298216	2276508	79.98%	11.181%
22	7.551	2016	2025	2048	rBV	222583	411671	14.46%	2.022%
23	8.027	2164	2173	2211	rBV3	381022	858196	30.15%	4.215%
24	8.506	2320	2322	2325	rBV4	1186	644	0.02%	0.003%
25	8.696	2380	2381	2384	rVB3	1077	523	0.02%	0.003%
26	8.718	2384	2388	2390	rBV3	1417	1172	0.04%	0.006%
27	8.780	2395	2407	2439	rBV	1219638	2015178	70.80%	9.897%
28	9.271	2558	2560	2562	rBV3	1258	723	0.03%	0.004%
29	9.316	2573	2574	2575	rBV2	924	295	0.01%	0.001%
30	9.429	2607	2609	2612	rVB4	1323	753	0.03%	0.004%
31	9.455	2612	2617	2620	rBV7	1491	1511	0.05%	0.007%
32	9.542	2642	2644	2648	rVB5	1426	1047	0.04%	0.005%
33	9.718	2696	2699	2701	rBV3	1416	1018	0.04%	0.005%
34	9.757	2707	2711	2714	rBV6	1085	799	0.03%	0.004%
35	9.789	2719	2721	2722	rBV2	941	257	0.01%	0.001%
36	9.815	2728	2729	2733	rBV4	1238	882	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081224\
 Data File : VV036901.D
 Acq On : 12 Aug 2024 13:29
 Operator : SY/MD
 Sample : P3533-11
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.857	2738	2742	2744	rBV5	1592	1248	0.04%	0.006%
38	9.943	2765	2769	2772	rBV6	1432	1125	0.04%	0.006%
39	9.956	2772	2773	2775	rBV2	635	342	0.01%	0.002%
40	10.037	2796	2798	2801	rBV4	669	343	0.01%	0.002%
41	10.056	2801	2804	2807	rVV5	1185	732	0.03%	0.004%
42	10.085	2811	2813	2815	rBV3	805	352	0.01%	0.002%
43	10.149	2822	2833	2863	rVB	623528	993526	34.91%	4.880%
44	10.349	2893	2895	2902	rBV7	1351	917	0.03%	0.005%
45	10.525	2947	2950	2951	rBV3	1849	1055	0.04%	0.005%
46	10.577	2964	2966	2969	rVB4	805	339	0.01%	0.002%
47	10.596	2969	2972	2978	rBV8	1862	1232	0.04%	0.006%
48	10.644	2986	2987	2991	rBV3	782	360	0.01%	0.002%
49	10.731	3012	3014	3016	rBV3	589	366	0.01%	0.002%
50	10.770	3023	3026	3027	rBV3	1244	648	0.02%	0.003%
51	10.828	3041	3044	3047	rBV4	1075	657	0.02%	0.003%
52	10.853	3049	3052	3053	rBV3	1333	744	0.03%	0.004%
53	10.931	3074	3076	3077	rBV2	607	161	0.01%	0.001%
54	10.966	3084	3087	3088	rBV3	1346	709	0.02%	0.003%
55	11.030	3105	3107	3109	rVB3	1437	628	0.02%	0.003%
56	11.075	3117	3121	3123	rBV6	562	456	0.02%	0.002%
57	11.104	3128	3130	3132	rBV2	784	381	0.01%	0.002%
58	11.181	3143	3154	3192	rBV	1250875	1979220	69.54%	9.721%
59	11.490	3248	3250	3251	rBV2	974	444	0.02%	0.002%
60	11.554	3259	3270	3298	rBV	1233050	1987543	69.83%	9.762%
61	11.914	3379	3382	3383	rBV3	1356	880	0.03%	0.004%
62	12.037	3416	3420	3422	rBV5	1210	1087	0.04%	0.005%
63	12.123	3445	3447	3448	rBV2	703	313	0.01%	0.002%
64	12.284	3493	3497	3504	rBV8	1343	1616	0.06%	0.008%
65	12.355	3513	3519	3522	rBV7	1914	2180	0.08%	0.011%
66	12.432	3539	3543	3548	rBV8	1456	1330	0.05%	0.007%
67	12.455	3548	3550	3552	rBV3	709	337	0.01%	0.002%
68	12.686	3621	3622	3623	rBV	797	272	0.01%	0.001%
69	12.805	3656	3659	3660	rBV3	831	554	0.02%	0.003%
70	12.895	3685	3687	3689	rVB3	1018	441	0.02%	0.002%
71	12.911	3690	3692	3695	rVB2	1495	751	0.03%	0.004%
72	12.934	3695	3699	3701	rBV4	1891	1275	0.04%	0.006%
73	13.049	3733	3735	3738	rVB4	1487	597	0.02%	0.003%
74	13.172	3771	3773	3776	rBV3	1224	688	0.02%	0.003%
75	13.336	3819	3824	3826	rBV5	1386	1153	0.04%	0.006%
76	13.384	3834	3839	3840	rBV4	1278	1183	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081224\
Data File : VV036901.D
Acq On : 12 Aug 2024 13:29
Operator : SY/MD
Sample : P3533-11
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AG6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Title : VOC Analysis

77	13.631	3914	3916	3918	rBV3	1182	606	0.02%	0.003%
78	14.152	4076	4078	4082	rBV3	2014	1549	0.05%	0.008%
79	14.303	4122	4125	4127	rBV4	1492	1026	0.04%	0.005%
80	14.451	4168	4171	4172	rBV3	1526	861	0.03%	0.004%
81	14.586	4211	4213	4214	rBV2	1577	656	0.02%	0.003%




Sum of corrected areas: 20360963

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081224\
Data File : VV036901.D
Acq On : 12 Aug 2024 13:29
Operator : SY/MD
Sample : P3533-11
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

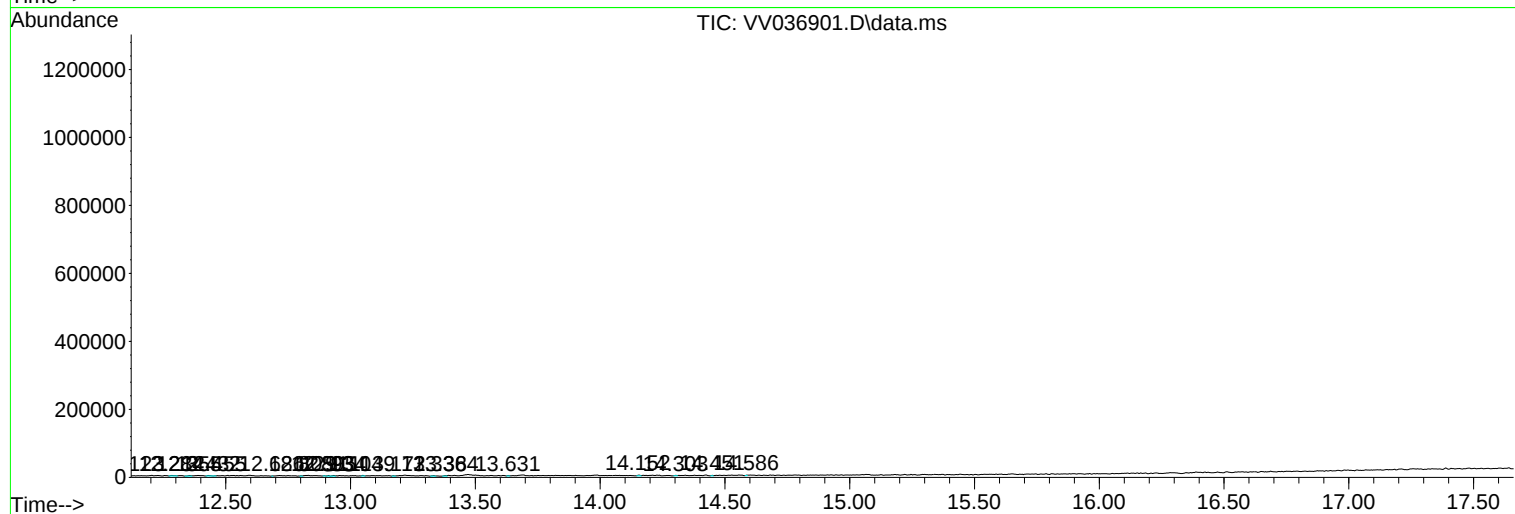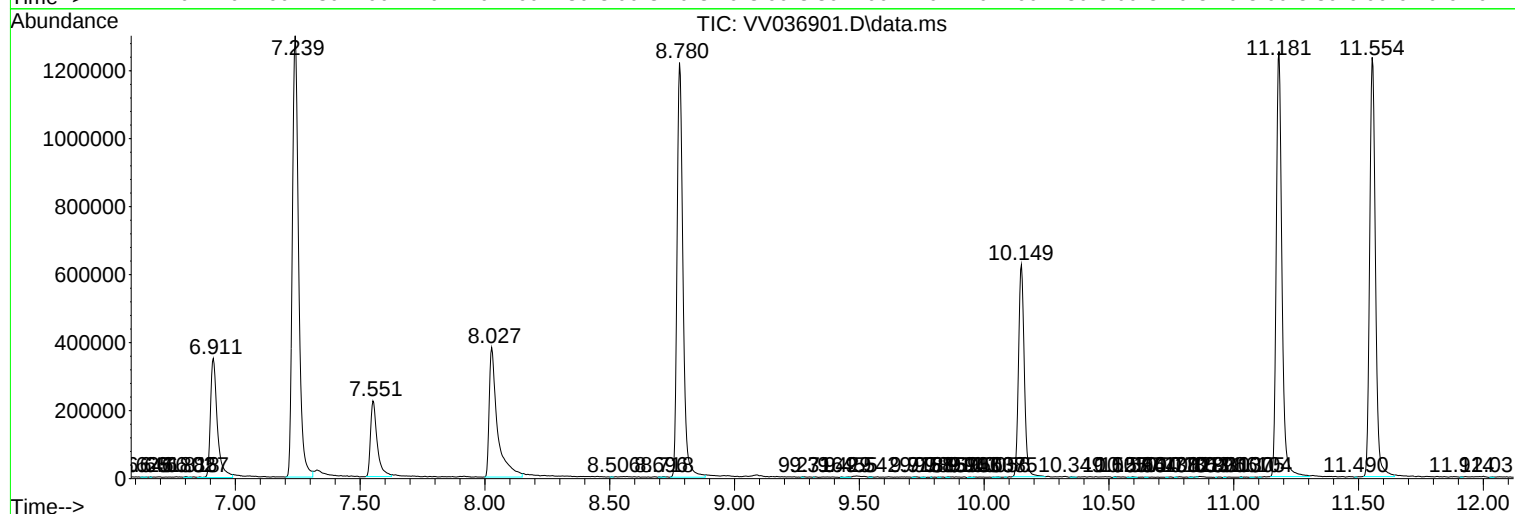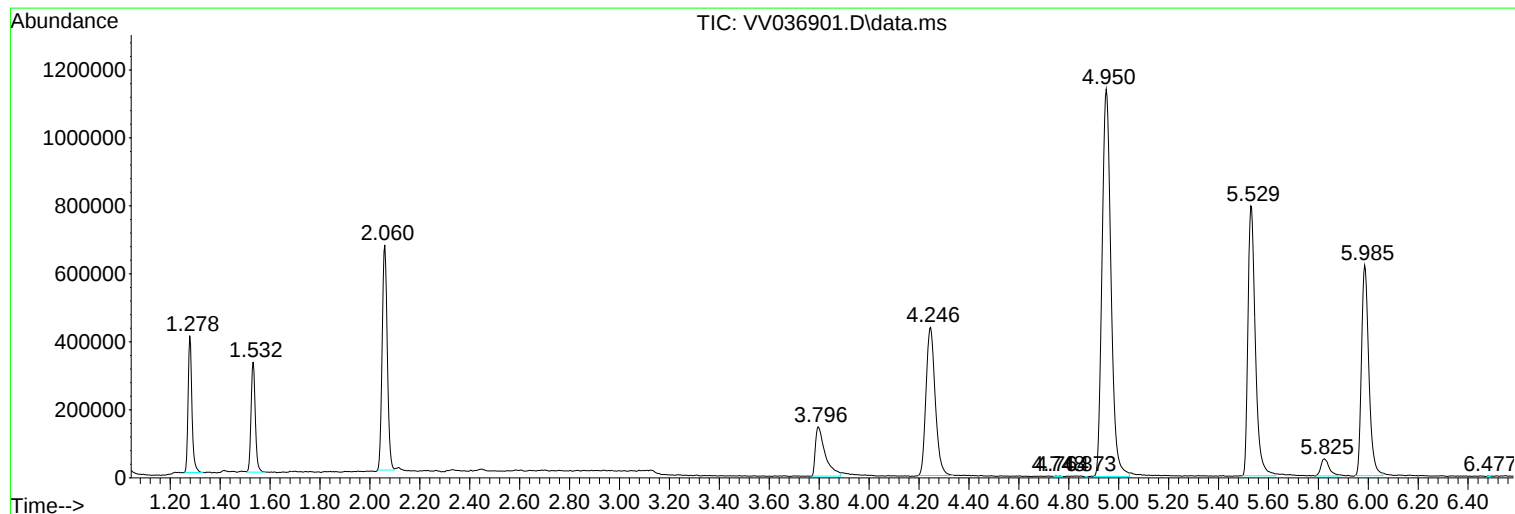

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081224\
Data File : VV036901.D
Acq On : 12 Aug 2024 13:29
Operator : SY/MD
Sample : P3533-11
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081224\
Data File : VV036901.D
Acq On : 12 Aug 2024 13:29
Operator : SY/MD
Sample : P3533-11
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc