

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081224\
 Data File : VV036910.D
 Acq On : 12 Aug 2024 17:08
 Operator : SY/MD
 Sample : P3498-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036910.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	225132	240058	10.34%	1.464%
2	1.532	147	153	166	rVB	227406	275250	11.85%	1.679%
3	2.060	309	317	330	rVB	378858	535776	23.07%	3.268%
4	3.674	816	819	822	rBV4	1747	1140	0.05%	0.007%
5	3.796	848	857	896	rBV	175382	492917	21.22%	3.006%
6	4.246	982	997	1029	rBV	381028	968613	41.71%	5.908%
7	4.619	1110	1113	1117	rBV5	1345	1455	0.06%	0.009%
8	4.654	1121	1124	1125	rBV3	1001	557	0.02%	0.003%
9	4.780	1160	1163	1164	rBV3	947	603	0.03%	0.004%
10	4.831	1176	1179	1181	rBV3	1796	1109	0.05%	0.007%
11	4.880	1192	1194	1197	rBV4	1203	831	0.04%	0.005%
12	4.896	1197	1199	1200	rBV2	1234	498	0.02%	0.003%
13	4.950	1201	1216	1243	rVV2	927840	2322533	100.00%	14.166%
14	5.532	1386	1397	1430	rBV	655278	1350769	58.16%	8.239%
15	5.825	1479	1488	1508	rBV2	33048	76466	3.29%	0.466%
16	5.986	1526	1538	1568	rBV	548712	1126655	48.51%	6.872%
17	6.404	1666	1668	1671	rBV4	1226	614	0.03%	0.004%
18	6.786	1784	1787	1788	rBV2	911	377	0.02%	0.002%
19	6.828	1794	1800	1802	rBV5	2298	1883	0.08%	0.011%
20	6.912	1812	1826	1852	rBV2	278227	535166	23.04%	3.264%
21	7.156	1898	1902	1905	rBV5	1658	1487	0.06%	0.009%
22	7.240	1918	1928	1956	rBV	862502	1529691	65.86%	9.330%
23	7.555	2017	2026	2055	rBV	175816	340940	14.68%	2.079%
24	8.027	2163	2173	2221	rBV2	471403	1040010	44.78%	6.343%
25	8.638	2359	2363	2366	rBV6	1836	1347	0.06%	0.008%
26	8.686	2373	2378	2381	rBV5	1755	1580	0.07%	0.010%
27	8.703	2381	2383	2385	rBV3	935	427	0.02%	0.003%
28	8.780	2397	2407	2433	rBV	935297	1560466	67.19%	9.518%
29	9.288	2563	2565	2566	rBV2	637	164	0.01%	0.001%
30	9.301	2567	2569	2570	rBV2	1093	411	0.02%	0.003%
31	9.439	2610	2612	2613	rVB2	703	224	0.01%	0.001%
32	9.497	2628	2630	2632	rVB3	1355	604	0.03%	0.004%
33	9.555	2642	2648	2651	rBV6	1550	1849	0.08%	0.011%
34	9.609	2664	2665	2666	rBV	780	263	0.01%	0.002%
35	9.696	2689	2692	2693	rBV3	1172	731	0.03%	0.004%
36	9.802	2722	2725	2729	rBV5	1130	988	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081224\
 Data File : VV036910.D
 Acq On : 12 Aug 2024 17:08
 Operator : SY/MD
 Sample : P3498-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.844	2736	2738	2741	rVB3	1197	713	0.03%	0.004%
38	9.860	2741	2743	2745	rBV2	1299	861	0.04%	0.005%
39	10.014	2787	2791	2796	rVB6	1810	1354	0.06%	0.008%
40	10.050	2796	2802	2804	rBV6	1112	966	0.04%	0.006%
41	10.072	2806	2809	2816	rBV8	1385	1095	0.05%	0.007%
42	10.149	2816	2833	2849	rBV	693809	1108606	47.73%	6.762%
43	10.407	2910	2913	2919	rBV6	1065	1136	0.05%	0.007%
44	10.474	2932	2934	2935	rVB	972	349	0.02%	0.002%
45	10.493	2935	2940	2943	rBV6	2488	1901	0.08%	0.012%
46	10.522	2946	2949	2955	rVB6	1595	1427	0.06%	0.009%
47	10.545	2955	2956	2959	rBV3	990	638	0.03%	0.004%
48	10.593	2966	2971	2973	rBV4	639	689	0.03%	0.004%
49	10.651	2987	2989	2991	rBV3	899	513	0.02%	0.003%
50	10.702	3003	3005	3008	rBV3	1424	686	0.03%	0.004%
51	10.731	3010	3014	3018	rBV4	1506	1196	0.05%	0.007%
52	10.841	3047	3048	3050	rVB2	664	212	0.01%	0.001%
53	10.979	3089	3091	3094	rVB4	1007	549	0.02%	0.003%
54	11.001	3095	3098	3099	rBV3	906	421	0.02%	0.003%
55	11.011	3099	3101	3102	rBV	1169	369	0.02%	0.002%
56	11.043	3107	3111	3114	rBV6	975	914	0.04%	0.006%
57	11.101	3123	3129	3131	rBV5	1192	1269	0.05%	0.008%
58	11.182	3143	3154	3178	rBV	884905	1405140	60.50%	8.570%
59	11.554	3260	3270	3302	rBV	884795	1435995	61.83%	8.758%
60	11.966	3396	3398	3399	rBV2	1033	354	0.02%	0.002%
61	12.075	3429	3432	3437	rBV6	1283	1094	0.05%	0.007%
62	12.442	3545	3546	3549	rVB2	823	261	0.01%	0.002%
63	12.477	3555	3557	3559	rVB3	1201	532	0.02%	0.003%
64	12.500	3559	3564	3566	rBV6	1527	1262	0.05%	0.008%
65	12.648	3608	3610	3613	rBV3	1273	803	0.03%	0.005%
66	12.780	3649	3651	3653	rBV4	1030	488	0.02%	0.003%
67	12.799	3653	3657	3660	rVV5	1425	1128	0.05%	0.007%
68	12.898	3685	3688	3690	rBV4	1040	632	0.03%	0.004%
69	12.963	3706	3708	3713	rVB5	1013	669	0.03%	0.004%
70	13.291	3808	3810	3812	rBV2	1506	791	0.03%	0.005%
71	13.358	3829	3831	3836	rVB6	1766	1138	0.05%	0.007%
72	13.384	3837	3839	3842	rVB4	1324	482	0.02%	0.003%
73	13.538	3885	3887	3892	rVB5	1819	930	0.04%	0.006%
74	13.651	3920	3922	3925	rBV3	1467	1035	0.04%	0.006%
75	13.767	3955	3958	3960	rBV2	1354	839	0.04%	0.005%
76	14.378	4145	4148	4153	rBV6	1438	1681	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081224\
Data File : VV036910.D
Acq On : 12 Aug 2024 17:08
Operator : SY/MD
Sample : P3498-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Title : VOC Analysis




Sum of corrected areas: 16395570

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081224\
Data File : VV036910.D
Acq On : 12 Aug 2024 17:08
Operator : SY/MD
Sample : P3498-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

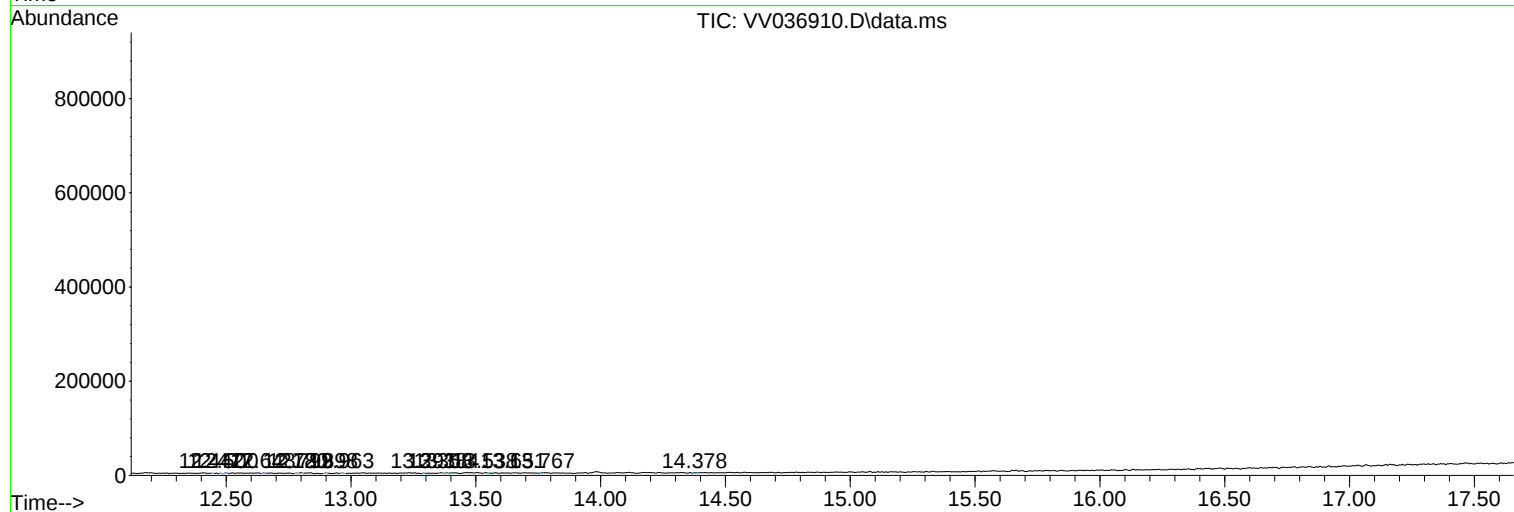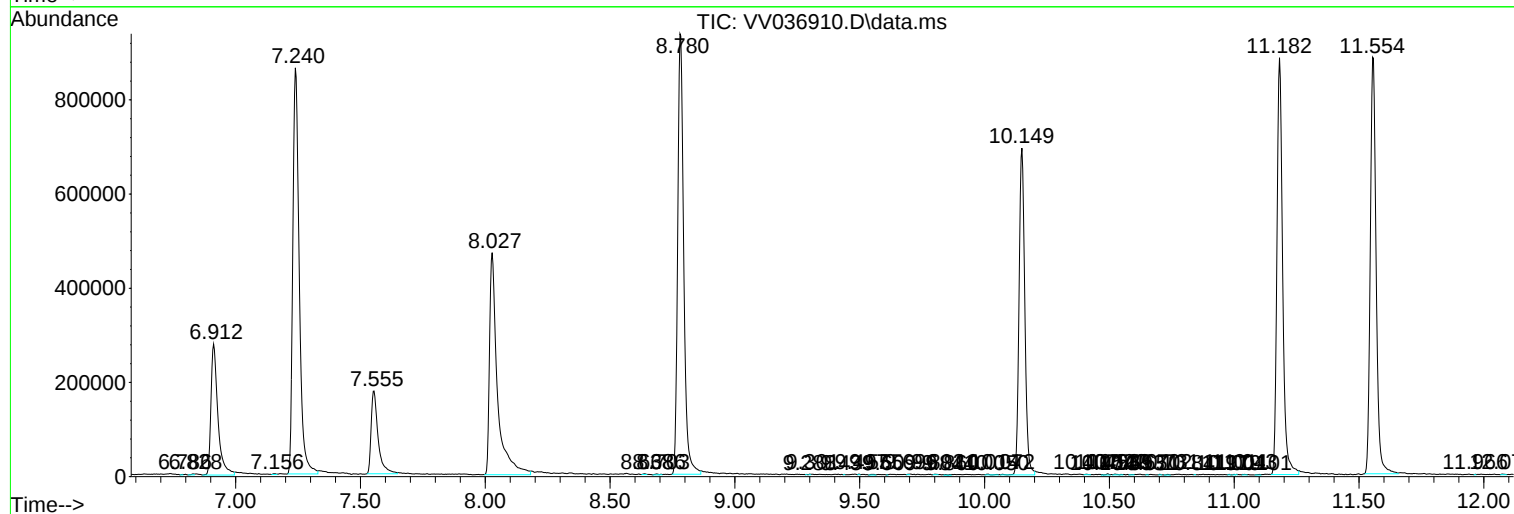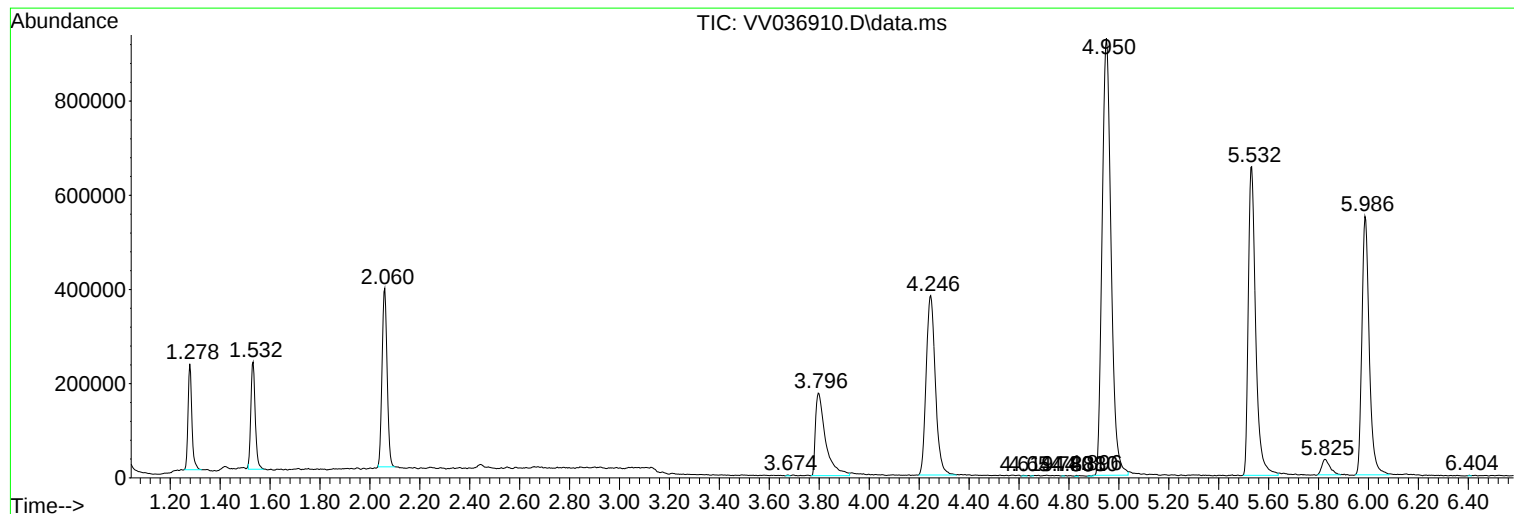

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081224\
Data File : VV036910.D
Acq On : 12 Aug 2024 17:08
Operator : SY/MD
Sample : P3498-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081224\
Data File : VV036910.D
Acq On : 12 Aug 2024 17:08
Operator : SY/MD
Sample : P3498-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
