


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081224\
Data File : VV036890.D
Acq On : 12 Aug 2024 08:57
Operator : SY/MD
Sample : BFB359
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB359

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Title : VOC Analysis
Last Update : Wed Aug 14 04:10:20 2024

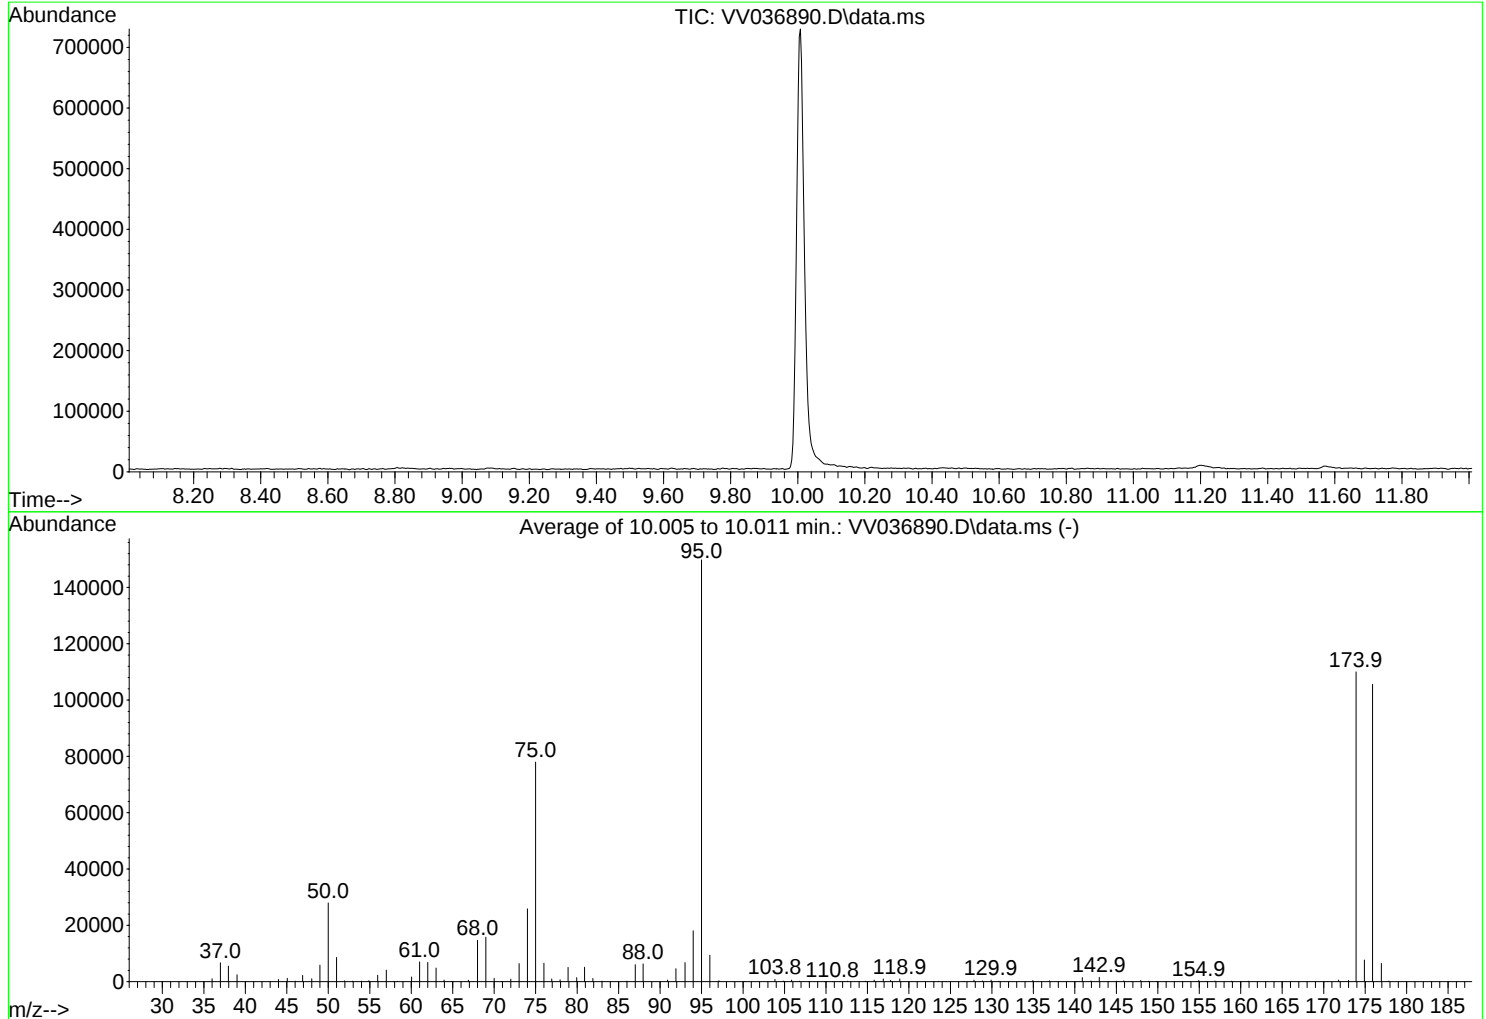

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	27936	PASS
75	95	30	80	52.1	77997	PASS
95	95	100	100	100.0	149803	PASS
96	95	5	9	6.2	9359	PASS
173	174	0.00	2	0.4	441	PASS
174	95	50	120	73.4	110024	PASS
175	174	5	9	7.0	7700	PASS
176	174	95	105	96.0	105581	PASS
177	176	5	10	6.2	6507	PASS

m/z	Abundance
35.20	102.0
36.00	209.0
37.30	123.0
37.80	162.0
38.70	164.0
39.10	150.0
39.90	502.0
41.00	300.0
41.90	252.0
43.00	239.0
44.00	1187.0
45.20	133.0
51.00	141.0
51.80	122.0
54.90	239.0
55.90	123.0
56.50	103.0
63.70	164.0
64.80	136.0
67.20	115.0
76.90	202.0
96.10	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB359

m/z	Abundance
36.00	1302.0
37.00	7240.0
38.00	6032.0
39.00	2609.0
40.00	447.0
41.00	252.0
41.90	194.0
43.00	340.0
44.00	2073.0
45.10	1438.0
46.10	212.0
46.90	2171.0
48.00	1055.0
49.00	5909.0
50.00	29072.0
51.00	9173.0
51.90	427.0
52.90	177.0
54.00	164.0
54.90	642.0
56.00	2620.0
57.00	4167.0
57.90	139.0
58.30	146.0
60.10	1685.0
61.00	7400.0
62.00	6976.0
63.00	5056.0
63.90	609.0
65.00	285.0
66.90	536.0
68.00	14900.0
69.00	15867.0
70.00	1318.0
70.90	122.0
72.00	927.0
73.00	6700.0
74.00	27168.0
75.00	79448.0
76.00	6733.0
77.00	1226.0
78.00	683.0
78.90	5058.0
80.00	1449.0
80.90	5253.0
81.90	1209.0
83.00	132.0
86.10	199.0
87.00	6272.0
87.90	6247.0
90.90	559.0
91.90	4707.0
93.00	6963.0
94.00	18112.0
95.00	152448.0
96.00	9781.0
97.10	468.0
100.20	107.0
103.80	807.0
104.90	240.0
105.90	614.0
106.80	165.0
107.90	108.0
109.80	153.0
112.60	151.0
114.70	184.0
115.80	630.0
116.90	1021.0
117.80	524.0
118.90	964.0
123.60	168.0
124.50	111.0
126.60	123.0
127.80	532.0
128.80	305.0
129.90	569.0
130.80	194.0
134.90	330.0
136.90	308.0
140.90	1464.0
141.90	214.0
143.00	1552.0
145.00	148.0
145.90	258.0
146.80	115.0
148.00	371.0
148.90	230.0
149.80	127.0
152.00	158.0
155.00	396.0
155.90	133.0
156.90	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB359

158.90	159.0
161.00	160.0
170.50	101.0
171.80	485.0
173.90	108720.0
174.90	7903.0
175.90	105520.0
177.00	6385.0
177.80	287.0

Instrument :
MSVOA_V
ClientSampleId :
BFB359

m/z	Abundance
36.00	1278.0
37.00	6907.0
38.00	5867.0
39.00	2680.0
40.00	418.0
41.00	243.0
41.90	123.0
43.00	376.0
44.00	2022.0
45.00	1339.0
46.00	193.0
46.90	2350.0
48.00	1046.0
49.00	6062.0
50.00	28736.0
51.00	8986.0
52.00	393.0
52.90	157.0
54.00	170.0
54.90	585.0
56.00	2527.0
57.00	4258.0
57.90	130.0
58.30	142.0
60.00	1692.0
61.00	7205.0
62.00	6951.0
63.00	4921.0
64.00	605.0
65.00	231.0
66.90	498.0
68.00	15225.0
69.00	16392.0
70.00	1220.0
72.00	962.0
73.00	6504.0
74.00	26696.0
75.00	80656.0
76.00	6850.0
77.00	1210.0
77.90	746.0
78.90	5296.0
79.90	1475.0
80.90	5355.0
81.90	1213.0
83.00	165.0
86.00	197.0
87.00	6146.0
87.90	6525.0
90.90	595.0
91.90	4754.0
93.00	7044.0
94.00	18688.0
95.00	154624.0
96.00	9644.0
97.10	354.0
103.80	900.0
104.80	237.0
105.80	578.0
106.80	135.0
110.10	133.0
110.80	110.0
112.60	154.0
114.70	190.0
115.80	588.0
116.90	936.0
117.80	464.0
118.90	1045.0
123.60	122.0
126.70	109.0
127.90	579.0
128.90	267.0
129.90	618.0
130.80	221.0
134.90	420.0
136.90	285.0
140.90	1483.0
141.90	263.0
142.90	1612.0
144.00	116.0
145.00	189.0
145.90	306.0
148.00	411.0
148.90	207.0
149.80	102.0
152.00	111.0
153.00	108.0
154.90	445.0
155.80	125.0
156.90	265.0
158.90	126.0
160.90	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB359

171.80	613.0
173.90	113648.0
174.90	7905.0
175.90	109432.0
177.00	6711.0
177.90	247.0

Instrument :
MSVOA_V
ClientSampleId :
BFB359

m/z	Abundance
36.00	1209.0
37.00	6022.0
38.00	5203.0
39.00	2482.0
40.00	430.0
41.00	229.0
43.00	357.0
44.00	1848.0
45.00	1140.0
46.00	198.0
46.90	2063.0
48.00	963.0
49.00	5606.0
50.00	26000.0
51.00	8067.0
52.10	428.0
52.90	130.0
54.00	119.0
54.90	468.0
56.00	2112.0
57.00	3809.0
57.90	124.0
58.40	111.0
60.00	1568.0
61.00	6421.0
62.00	6528.0
63.00	4574.0
64.00	516.0
64.80	210.0
65.90	101.0
66.90	435.0
68.00	13902.0
69.00	15188.0
70.00	1000.0
72.00	904.0
73.00	6035.0
74.00	23720.0
75.00	73888.0
76.00	6067.0
77.00	1070.0
77.90	687.0
78.90	4868.0
79.90	1392.0
80.90	4790.0
81.90	1013.0
83.00	182.0
85.90	221.0
87.00	5742.0
88.00	6137.0
90.90	644.0
91.90	4310.0
93.00	6218.0
94.00	17408.0
95.00	142336.0
96.00	9022.0
97.10	248.0
103.90	770.0
104.80	231.0
105.80	572.0
106.80	145.0
110.10	112.0
110.80	147.0
111.70	137.0
112.60	145.0
114.80	183.0
115.80	492.0
116.90	909.0
117.80	397.0
118.90	920.0
123.00	121.0
127.90	583.0
128.90	264.0
129.90	564.0
130.90	200.0
135.00	435.0
137.00	292.0
140.00	116.0
140.90	1377.0
142.00	271.0
142.90	1453.0
144.10	141.0
145.00	204.0
145.90	308.0
147.90	356.0
148.80	129.0
149.90	110.0
153.00	174.0
154.90	440.0
155.80	117.0
156.90	309.0
158.80	104.0
159.00	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB359

160.80	136.0
171.80	667.0
173.00	1324.0
173.90	107704.0
174.90	7291.0
175.90	101792.0
176.90	6424.0
177.90	195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB359