


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081318\
Data File : VV006998.D
Acq On : 13 Aug 2018 09:04
Operator : SY/MD
Sample : BFB83
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB83

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Aug 14 05:35:33 2018

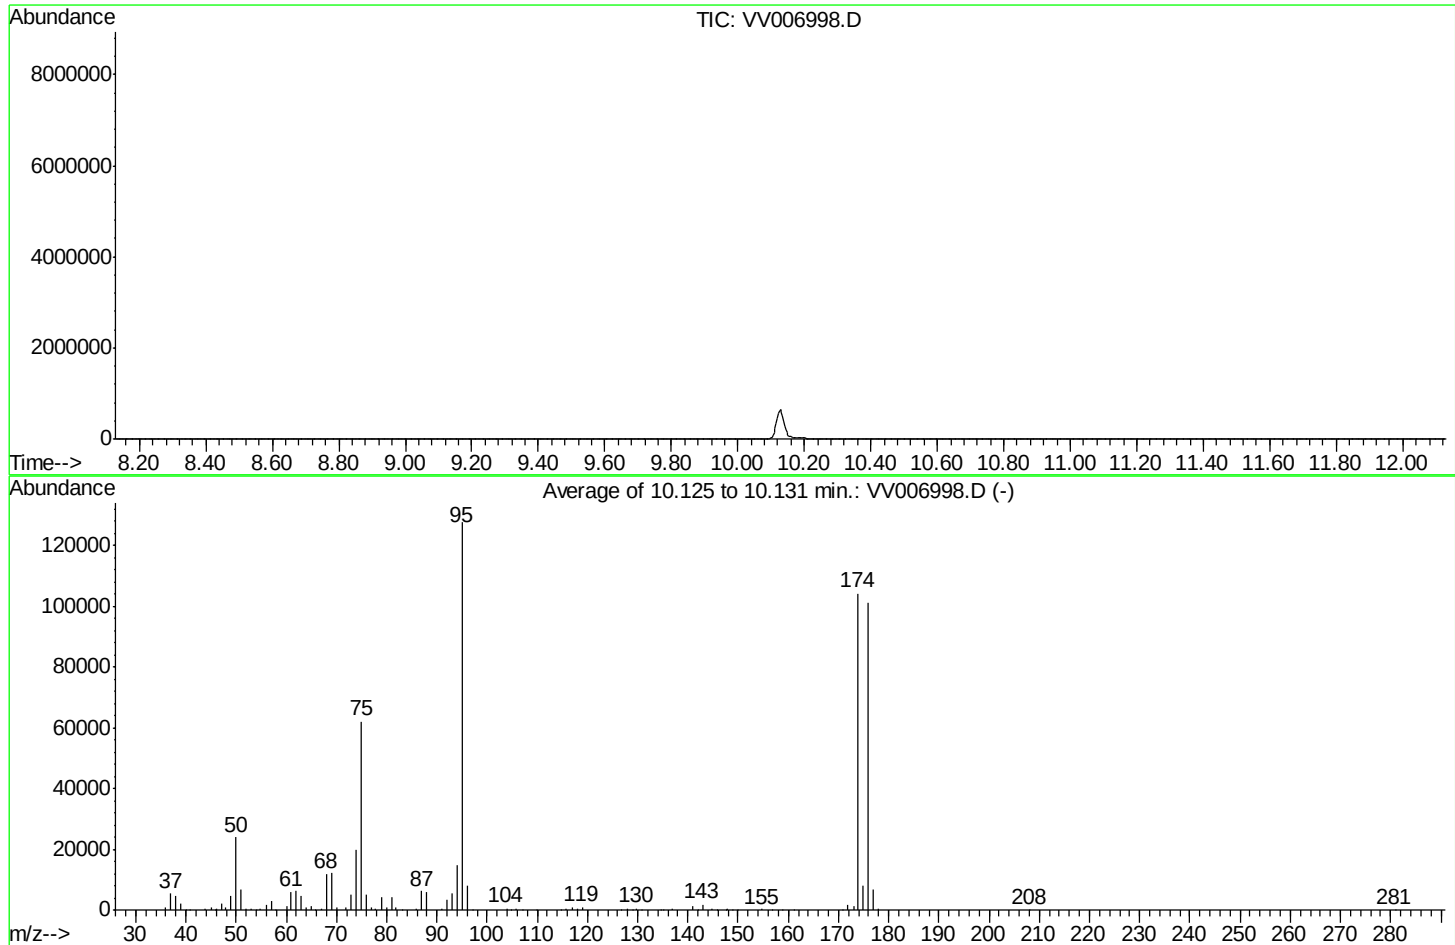

AutoFind: Scans 2872, 2873, 2874; Background Corrected with Scan 2857

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	23968	PASS
75	95	30	80	48.7	62106	PASS
95	95	100	100	100.0	127616	PASS
96	95	5	9	6.4	8203	PASS
173	174	0.00	2	1.2	1267	PASS
174	95	50	120	81.7	104261	PASS
175	174	5	9	7.5	7825	PASS
176	174	95	101	97.0	101117	PASS
177	176	5	9	6.6	6701	PASS

Scan 2857 (10.077 min): VV006998.D
BFB83

m/z	Abundance
37.80	122.0
38.80	152.0
40.00	570.0
42.00	203.0
42.90	118.0
43.90	1302.0
44.80	116.0
54.80	148.0
73.00	119.0
77.10	150.0
98.10	148.0
207.00	295.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
36.00	942.0
37.00	5436.0
38.00	5006.0
39.00	2119.0
39.90	628.0
40.70	178.0
43.90	1861.0
45.00	952.0
45.90	226.0
46.20	268.0
47.00	2195.0
47.90	776.0
49.00	4933.0
50.00	24616.0
51.00	7534.0
52.00	275.0
52.90	205.0
53.90	163.0
54.90	483.0
56.00	1633.0
57.00	3043.0
57.80	139.0
60.00	1184.0
61.00	6005.0
62.00	6553.0
63.00	4875.0
64.00	1067.0
65.00	1337.0
65.90	105.0
67.00	444.0
68.00	12456.0
69.00	13092.0
70.00	940.0
71.90	717.0
73.00	5702.0
74.00	20976.0
75.00	63912.0
76.00	5424.0
76.90	814.0
77.80	592.0
78.90	4163.0
79.90	1088.0
80.90	4195.0
81.90	910.0
83.00	105.0
86.00	251.0
86.90	6722.0
87.90	5937.0
91.00	434.0
91.90	3661.0
93.00	5487.0
94.00	15076.0
95.00	130200.0
96.00	8272.0
97.00	190.0
103.90	519.0
105.90	490.0
106.90	103.0
115.80	500.0
116.90	954.0
118.00	370.0
118.90	896.0
126.70	103.0
127.80	542.0
128.90	231.0
129.90	443.0
130.70	149.0
134.70	211.0
136.90	209.0
140.90	1170.0
141.80	172.0
143.00	1756.0
144.80	570.0
145.90	149.0
147.70	330.0
148.80	106.0
154.80	322.0
156.80	203.0
158.70	191.0
161.00	183.0
170.90	220.0
171.90	1728.0
173.00	1350.0
173.90	102992.0
174.90	8140.0
175.90	100392.0
176.90	6468.0
177.90	207.0
207.10	212.0
280.90	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
35.90	997.0
37.00	5442.0
38.00	4951.0
39.00	2123.0
40.00	735.0
40.70	207.0
43.10	138.0
43.90	1747.0
45.00	987.0
46.20	247.0
47.00	2034.0
47.90	780.0
49.00	4949.0
50.00	24880.0
51.00	7076.0
51.90	288.0
52.90	255.0
53.90	157.0
54.90	477.0
56.00	1645.0
57.00	3075.0
57.90	139.0
60.00	1164.0
61.00	6225.0
62.00	6414.0
63.00	4734.0
64.00	1019.0
65.00	1351.0
65.90	145.0
67.00	510.0
68.00	12333.0
69.00	12655.0
70.00	949.0
71.90	825.0
73.00	5210.0
74.00	20376.0
75.00	64040.0
76.00	5082.0
76.90	835.0
77.80	507.0
78.90	4257.0
79.90	1038.0
80.90	4248.0
81.90	954.0
83.10	131.0
86.00	237.0
86.90	6417.0
87.90	6003.0
91.00	510.0
92.00	3643.0
93.00	5561.0
94.00	15181.0
95.00	131648.0
96.00	8453.0
97.00	193.0
103.90	531.0
104.80	130.0
105.90	487.0
107.00	123.0
109.80	106.0
114.80	135.0
115.80	425.0
116.90	940.0
117.90	339.0
118.90	923.0
127.90	506.0
129.00	216.0
129.90	509.0
130.70	182.0
134.70	199.0
136.80	233.0
140.90	1211.0
141.80	185.0
142.90	1798.0
144.80	653.0
145.90	163.0
147.90	370.0
149.80	107.0
154.80	327.0
156.70	242.0
158.70	188.0
161.00	162.0
170.90	200.0
171.90	1800.0
173.00	1314.0
173.90	107712.0
174.90	8157.0
175.90	104664.0
176.90	6839.0
177.90	230.0
207.10	236.0
280.90	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
35.90	998.0
37.00	5078.0
38.00	4597.0
39.00	2095.0
40.00	742.0
40.70	157.0
43.00	170.0
43.90	1661.0
45.00	954.0
46.20	211.0
47.00	1711.0
47.80	782.0
49.00	4509.0
50.00	22408.0
51.00	6165.0
52.00	260.0
52.90	305.0
53.90	142.0
54.90	421.0
56.00	1480.0
57.00	2929.0
57.80	142.0
60.00	1126.0
61.00	5654.0
62.00	5801.0
63.00	4432.0
64.00	904.0
65.00	1326.0
65.80	147.0
67.00	469.0
68.00	11212.0
69.00	11285.0
70.00	946.0
71.90	797.0
72.90	4408.0
74.00	18400.0
75.00	58368.0
76.00	4286.0
76.90	847.0
77.80	487.0
78.90	3915.0
79.90	1016.0
80.90	3771.0
81.90	954.0
83.10	117.0
85.90	190.0
86.90	5570.0
87.90	5479.0
90.90	471.0
92.00	3302.0
93.00	5126.0
94.00	13775.0
95.00	121000.0
96.00	7886.0
97.10	198.0
103.90	523.0
104.80	180.0
105.80	432.0
107.00	117.0
114.80	167.0
115.80	405.0
116.90	787.0
117.90	308.0
118.90	872.0
127.90	417.0
129.00	216.0
129.80	539.0
130.80	215.0
135.00	201.0
136.80	234.0
140.90	1106.0
141.90	129.0
143.00	1673.0
144.80	579.0
145.90	171.0
147.90	389.0
149.80	131.0
154.80	278.0
156.70	223.0
158.70	141.0
161.00	127.0
170.80	156.0
171.90	1699.0
173.10	1137.0
173.90	102080.0
174.90	7180.0
175.90	98296.0
176.90	6797.0
177.90	243.0
207.10	272.0
208.10	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83