


Data File : VV012215.D
Acq On : 13 Aug 2019 15:00
Operator : SY/MD
Sample : VSTD00136
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD00136

Manual Integrations APPROVED

MMDadoda
8/14/2019 10:33:32 AM

Quant Time: Aug 14 02:12:17 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 14 02:01:27 2019
Response via : Initial Calibration

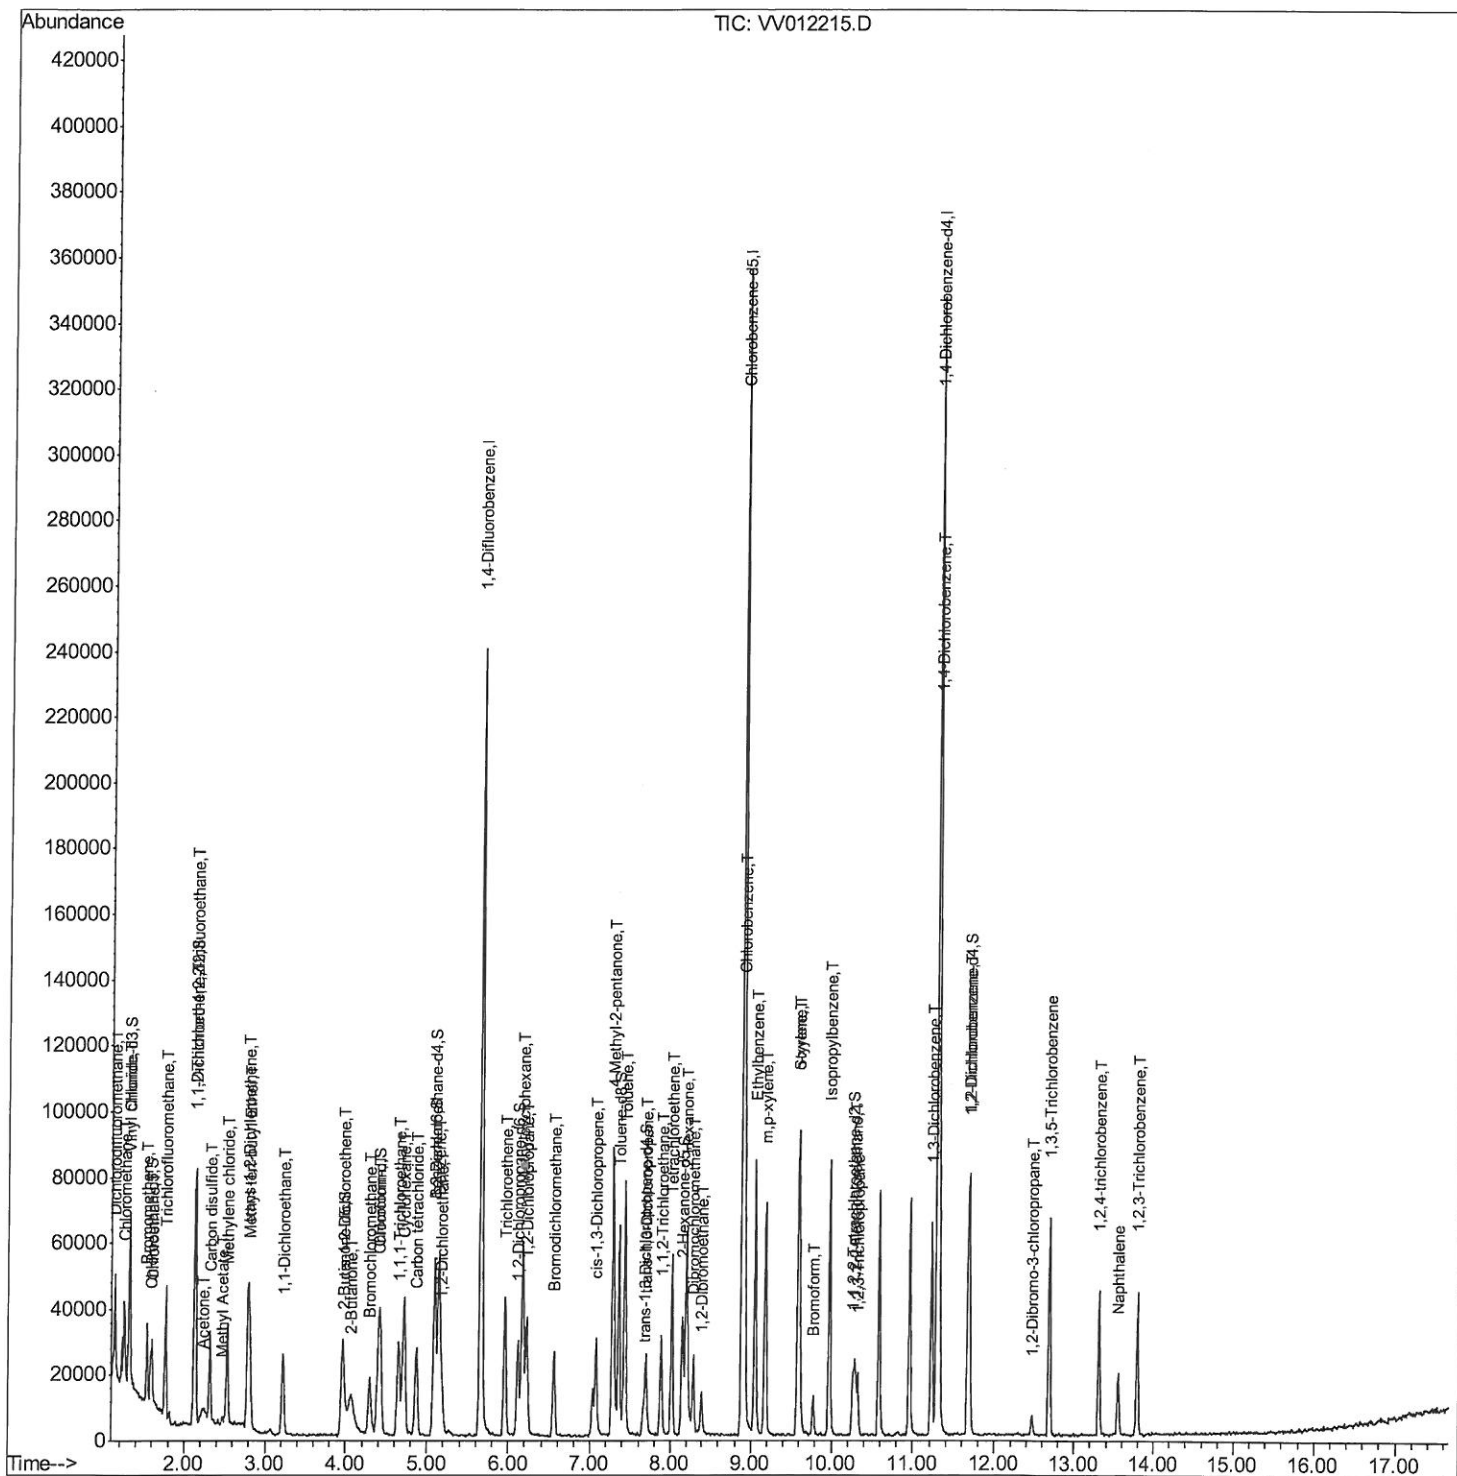

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
Quantitation Report (Qedit)




Data File : VV012215.D
Acq On : 13 Aug 2019 15:00
Operator : SY/MD
Sample : VSTD00136
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD00136

Manual Integrations
APPROVED

MMDadoda
8/14/2019 10:33:32 AM

Quant Time: Aug 14 02:04:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 14 02:01:27 2019
Response via : Initial Calibration

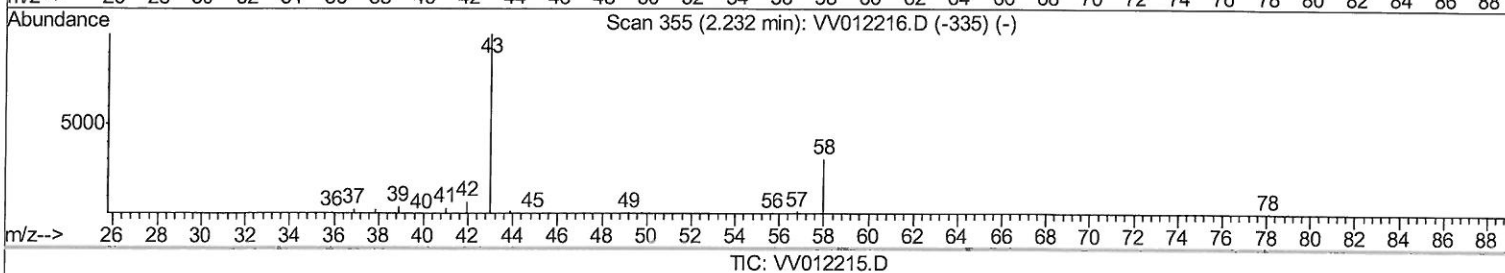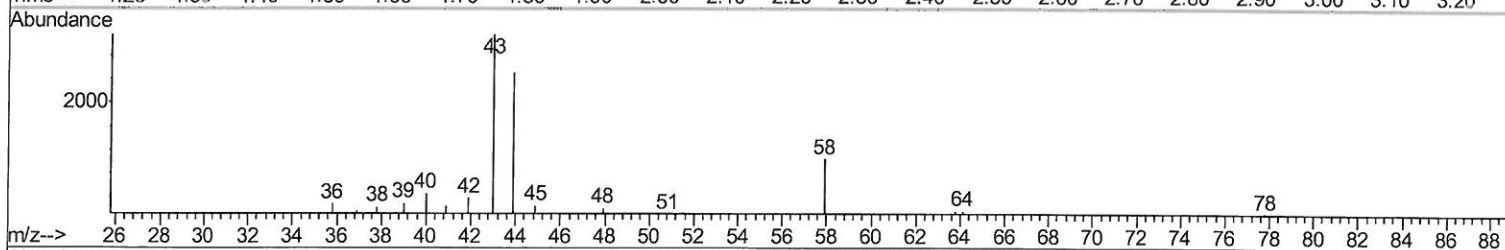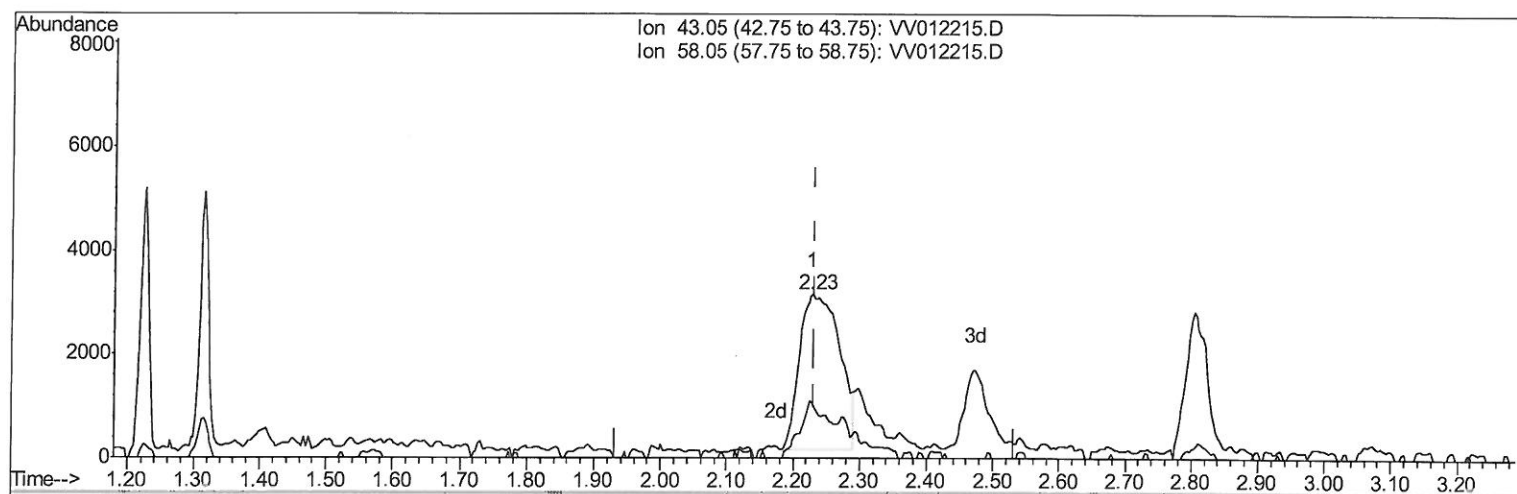

(13) Acetone (T)

2.228min (-0.003) 9.13ug/L

response 12636

Ion	Exp%	Act%
43.05	100	100
58.05	29.70	17.02
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
Quantitation Report (Qedit)




Data File : VV012215.D
Acq On : 13 Aug 2019 15:00
Operator : SY/MD
Sample : VSTD00136
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD00136

Manual Integrations
APPROVED

MMDadoda
8/14/2019 10:33:32 AM

Quant Time: Aug 14 02:04:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 14 02:01:27 2019
Response via : Initial Calibration

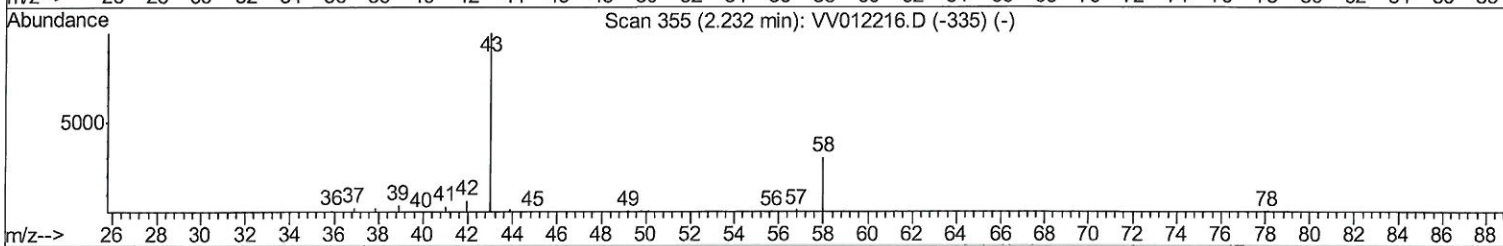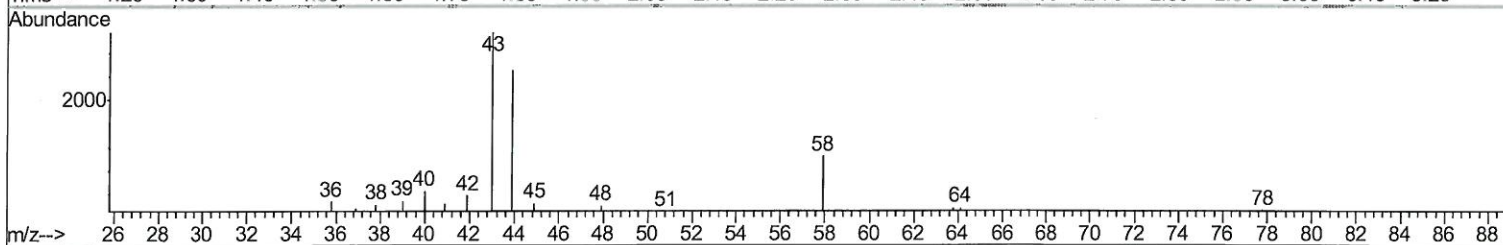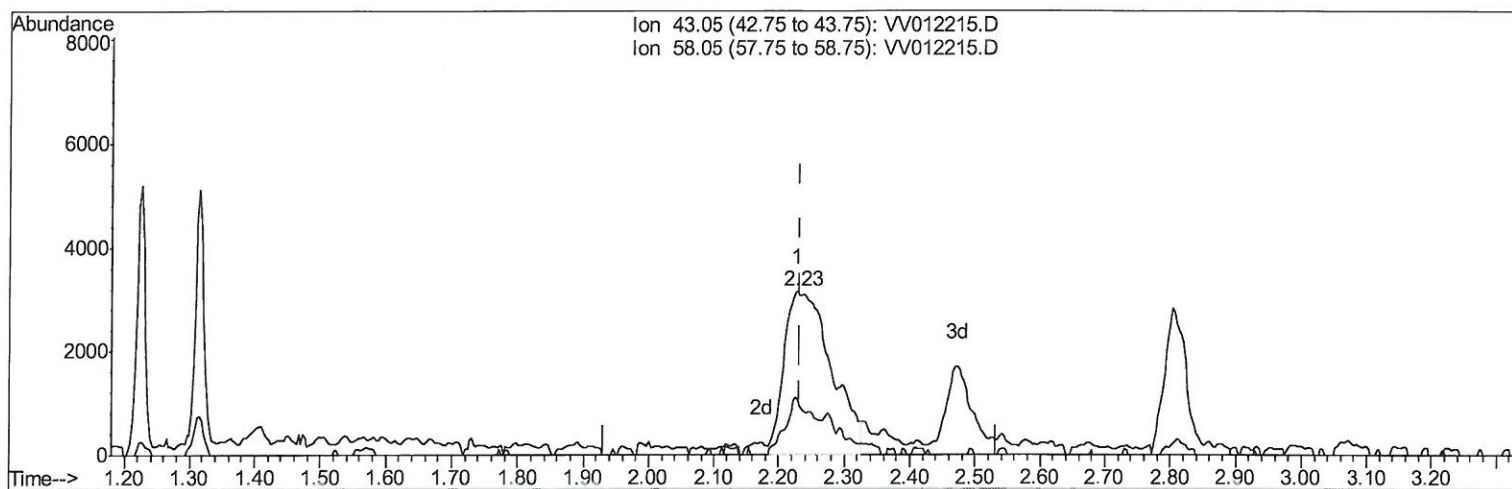

TIC: VV012215.D

(13) Acetone (T)

2.228min (-0.003) 11.37ug/L m

response 15740

Ion	Exp%	Act%
43.05	100	100
58.05	29.70	13.67
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
8/22/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
Quantitation Report (Qedit)




Data File : VV012215.D
Acq On : 13 Aug 2019 15:00
Operator : SY/MD
Sample : VSTD00136
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD00136

Manual Integrations
APPROVED

MMDadoda
8/14/2019 10:33:32 AM

Quant Time: Aug 14 02:04:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 14 02:01:27 2019
Response via : Initial Calibration

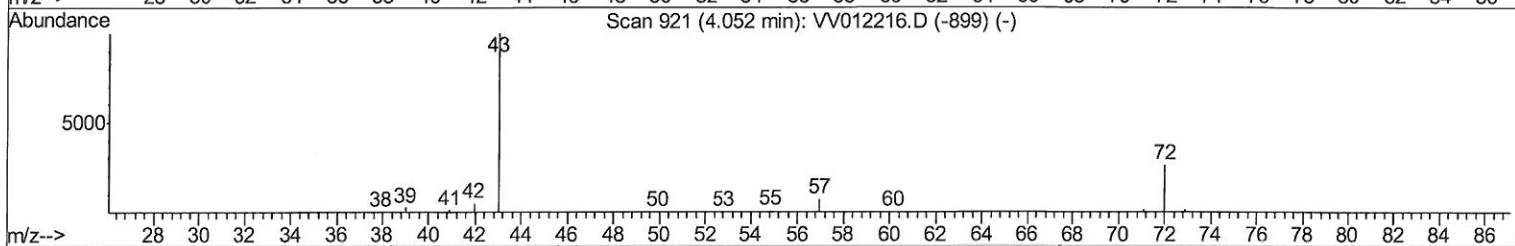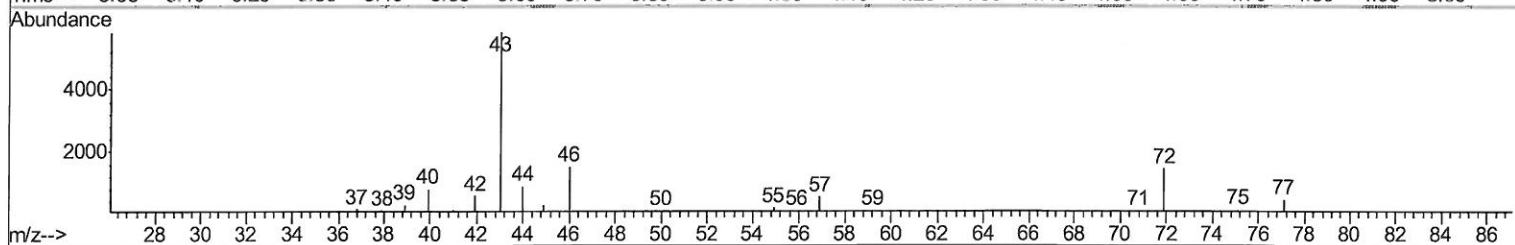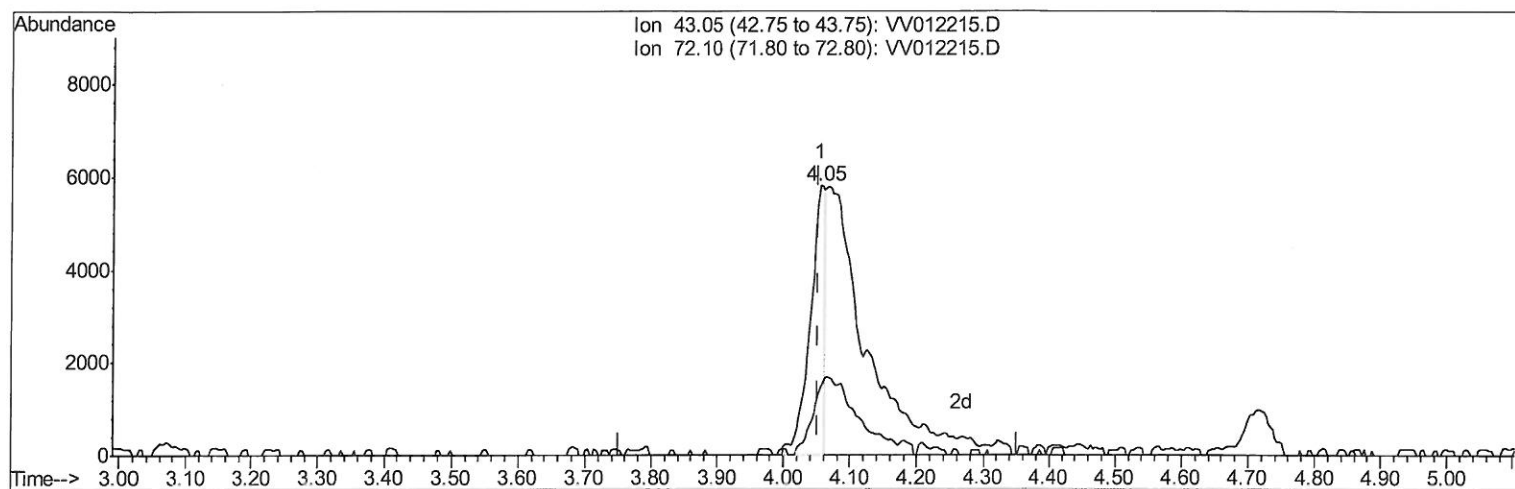

TIC: VV012215.D

(21) 2-Butanone (T)

4.055min (+0.003) 3.56ug/L

response 8984

Ion	Exp%	Act%
43.05	100	100
72.10	25.80	85.72#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
Quantitation Report (Qedit)




Data File : VV012215.D
Acq On : 13 Aug 2019 15:00
Operator : SY/MD
Sample : VSTD00136
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD00136

Manual Integrations
APPROVED

MMDadoda
8/14/2019 10:33:32 AM

Quant Time: Aug 14 02:04:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 14 02:01:27 2019
Response via : Initial Calibration

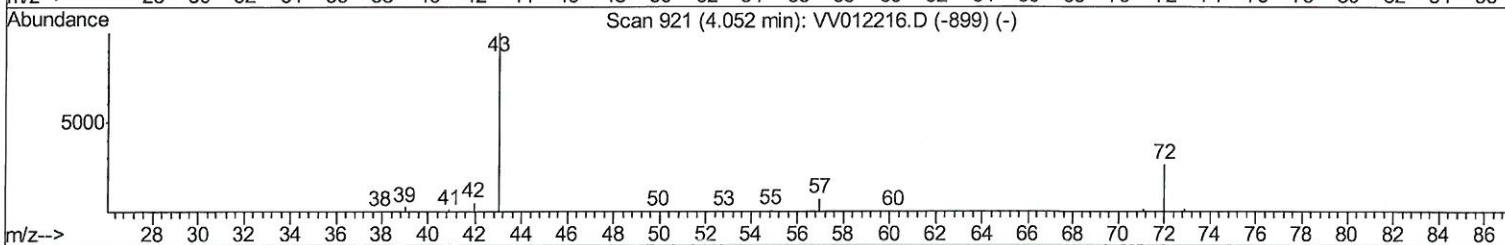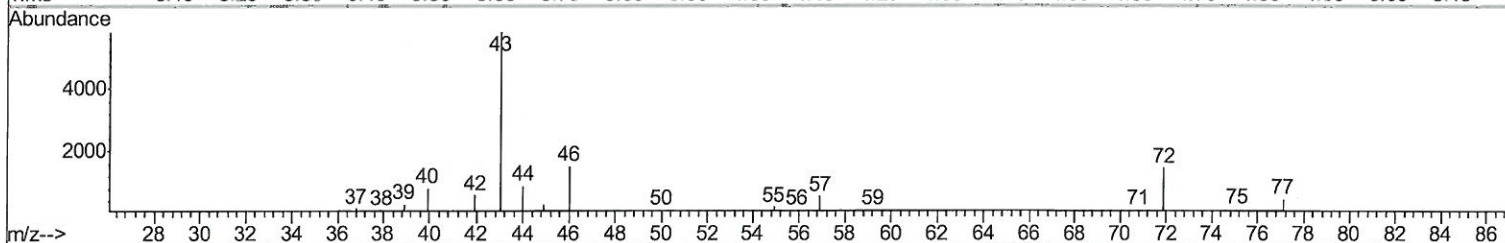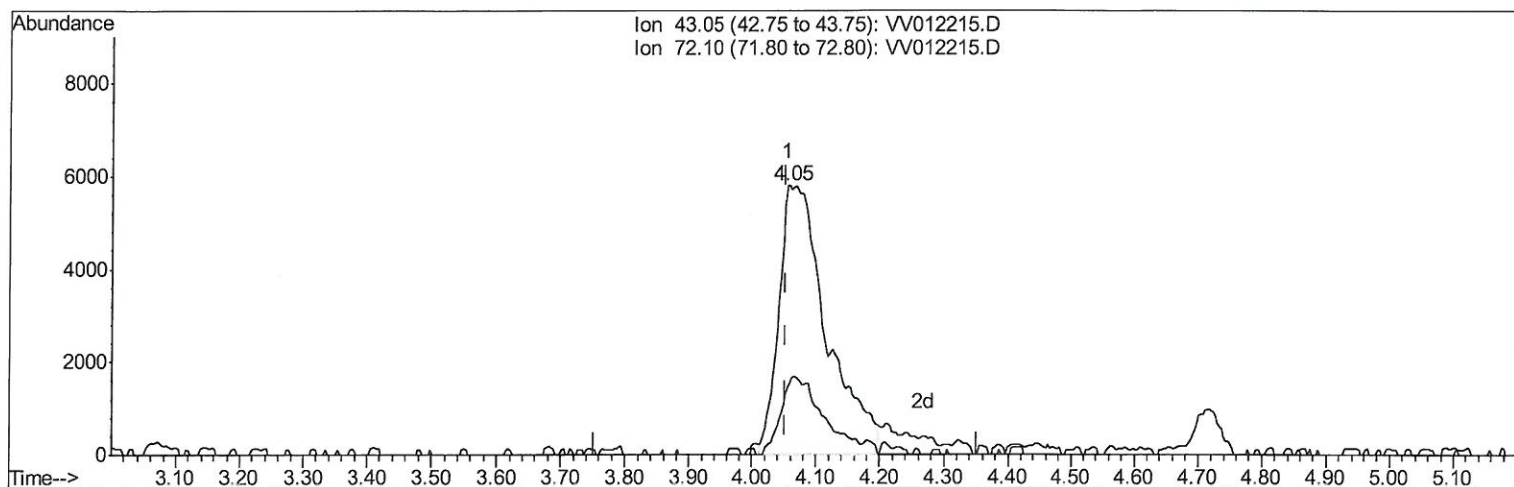

TIC: VV012215.D

(21) 2-Butanone (T)

4.055min (+0.003) 11.96ug/L m

response 30165

Ion Exp% Act%

43.05 100 100

72.10 25.80 25.53

0.00 0.00 0.00

0.00 0.00 0.00

7 MD
8/20/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
Quantitation Report (QT Reviewed)

Data File : VV012215.D
Acq On : 13 Aug 2019 15:00
Operator : SY/MD
Sample : VSTD00136
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD00136

Manual Integrations
APPROVED

MMDadoda
8/14/2019 10:33:32 AM

Quant Time: Aug 14 02:12:17 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 14 02:01:27 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.66	114	202597	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	196999	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	93388	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	12085	1.33	ug/L	0.00
7) Chloroethane-d5	1.58	69	9363	1.35	ug/L	0.00
11) 1,1-Dichloroethene-d2	2.13	63	18185	1.03	ug/L	0.00
20) 2-Butanone-d5	3.99	46	23553	10.24	ug/L	0.02
24) Chloroform-d	4.40	84	23922	0.97	ug/L	0.00
26) 1,2-Dichloroethane-d4	5.08	65	11030	0.88	ug/L	0.00
32) Benzene-d6	5.09	84	44994	0.93	ug/L	0.00
36) 1,2-Dichloropropane-d6	6.12	67	13150	1.01	ug/L	0.00
41) Toluene-d8	7.36	98	38750	0.80	ug/L	0.00
43) trans-1,3-Dichloropropene-	7.67	79	5418	0.85	ug/L	0.00
46) 2-Hexanone-d5	8.14	63	12354	6.01	ug/L	0.00
57) 1,1,2,2-Tetrachloroethane-	10.26	84	9117	0.87	ug/L	0.00
64) 1,2-Dichlorobenzene-d4	11.67	152	14693	0.88	ug/L	0.00

Target Compounds

					Qvalue
2) Dichlorodifluoromethane	1.14	85	18209	0.943	ug/L 98
3) Chloromethane	1.25	50	16851	1.625	ug/L 95
5) Vinyl chloride	1.32	62	17545	1.515	ug/L 98
6) Bromomethane	1.53	94	9567	1.443	ug/L 97
8) Chloroethane	1.60	64	9794	1.505	ug/L 92
9) Trichlorofluoromethane	1.77	101	22130	1.104	ug/L 99
10) 1,1,2-Trichloro-1,2,2-trif	2.14	101	10328	1.120	ug/L 97
12) 1,1-Dichloroethene	2.14	96	9276	1.094	ug/L 97
13) Acetone	2.23	43	15740m	11.368	ug/L 97
14) Carbon disulfide	2.31	76	30009	1.257	ug/L 99
15) Methyl Acetate	2.47	43	3712	1.194	ug/L 95
16) Methylene chloride	2.53	84	12547	1.379	ug/L 91
17) Methyl tert-butyl Ether	2.81	73	29323	1.034	ug/L 96
18) trans-1,2-Dichloroethene	2.78	96	14439	1.163	ug/L 95
19) 1,1-Dichloroethane	3.22	63	24548	1.168	ug/L 97
21) 2-Butanone	4.05	43	30165m	11.958	ug/L 96
22) cis-1,2-Dichloroethene	3.96	96	14086	1.021	ug/L 96
23) Bromochloromethane	4.30	128	6321	0.981	ug/L 98
25) Chloroform	4.42	83	29540	1.135	ug/L 96
27) 1,2-Dichloroethane	5.18	62	15142	0.983	ug/L 99
29) 1,1,1-Trichloroethane	4.65	97	22305	0.911	ug/L 99
30) Cyclohexane	4.71	56	20609	1.092	ug/L 99
31) Carbon tetrachloride	4.87	117	19896	0.850	ug/L 96
33) Benzene	5.14	78	53455	1.053	ug/L 100
34) Trichloroethene	5.96	95	14710	1.001	ug/L 97
35) Methylcyclohexane	6.17	83	20983	0.907	ug/L 95
37) 1,2-Dichloropropane	6.22	63	13334	1.162	ug/L 99
38) Bromodichloromethane	6.55	83	17360	0.952	ug/L 96
39) cis-1,3-Dichloropropene	7.07	75	16410	0.839	ug/L 96
40) 4-Methyl-2-pentanone	7.28	43	65631	10.120	ug/L 99

7 MD
8/20/19

7 MD
8/20/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
Quantitation Report (QT Reviewed)

Data File : VV012215.D
Acq On : 13 Aug 2019 15:00
Operator : SY/MD
Sample : VSTD00136
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD00136

Manual Integrations
APPROVED

MMDadoda
8/14/2019 10:33:32 AM

Quant Time: Aug 14 02:12:17 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 14 02:01:27 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
42) Toluene	7.43	91	54482	0.936	ug/L	96
44) trans-1,3-Dichloropropene	7.69	75	13837	0.902	ug/L	100
45) 1,1,2-Trichloroethane	7.88	97	8560	0.927	ug/L	98
47) Tetrachloroethene	8.02	164	12161	0.885	ug/L	95
48) 2-Hexanone	8.19	43	44628	9.780	ug/L	99
49) Dibromochloromethane	8.29	129	10495	0.793	ug/L	90
50) 1,2-Dibromoethane	8.40	107	8805	0.969	ug/L	92
51) Chlorobenzene	8.92	112	37281	0.957	ug/L	99
52) Ethylbenzene	9.05	91	56860	0.876	ug/L	99
53) m,p-xylene	9.18	106	21027	0.828	ug/L	94
54) o-xylene	9.59	106	19560	0.800	ug/L	91
55) Styrene	9.60	104	31710	0.777	ug/L	99
56) Isopropylbenzene	9.97	105	52093	0.776	ug/L	99
58) 1,1,2,2-Tetrachloroethane	10.29	83	9831	0.958	ug/L #	98
59) 1,2,3-Trichloropropane	10.32	75	7604	0.968	ug/L	90
61) Bromoform	9.77	173	5362	0.760	ug/L	98
62) 1,3-Dichlorobenzene	11.22	146	28001	0.947	ug/L	98
63) 1,4-Dichlorobenzene	11.31	146	28429	0.962	ug/L	99
65) 1,2-Dichlorobenzene	11.69	146	25496	0.933	ug/L	98
66) 1,2-Dibromo-3-chloropropan	12.48	75	1744	1.012	ug/L #	83
67) 1,3,5-Trichlorobenzene	12.69	180	20653	0.840	ug/L	99
68) 1,2,4-trichlorobenzene	13.31	180	13910	0.696	ug/L	97
69) Naphthalene	13.55	128	15709	0.493	ug/L	98
70) 1,2,3-Trichlorobenzene	13.79	180	13648	0.714	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed