

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
 Data File : VV012221.D
 Acq On : 13 Aug 2019 18:12
 Operator : SY/MD
 Sample : K4337-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ2

Quant Time: Aug 14 03:58:57 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 14 02:48:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	198739	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	193061	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	81197	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	60613	4.95	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.00%
7) Chloroethane-d5	1.58	69	48293	5.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.20%
11) 1,1-Dichloroethene-d2	2.13	63	81587	4.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.40%
20) 2-Butanone-d5	3.95	46	156474	59.17	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.34%
24) Chloroform-d	4.40	84	121541	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.20%
26) 1,2-Dichloroethane-d4	5.08	65	60501	5.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.40%
32) Benzene-d6	5.10	84	250030	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.40%
36) 1,2-Dichloropropane-d6	6.12	67	75072	5.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.40%
41) Toluene-d8	7.36	98	213800	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
43) trans-1,3-Dichloropropene-	7.67	79	27786	5.04	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	100.80%
46) 2-Hexanone-d5	8.14	63	90445	51.17	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.34%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	51293	5.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	76877	5.59	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.80%


Target Compounds					Qvalue
13) Acetone	2.21	43	18157	11.018 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
Data File : VV012221.D
Acq On : 13 Aug 2019 18:12
Operator : SY/MD
Sample : K4337-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ2

Quant Time: Aug 14 03:58:57 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 14 02:48:55 2019
Response via : Initial Calibration

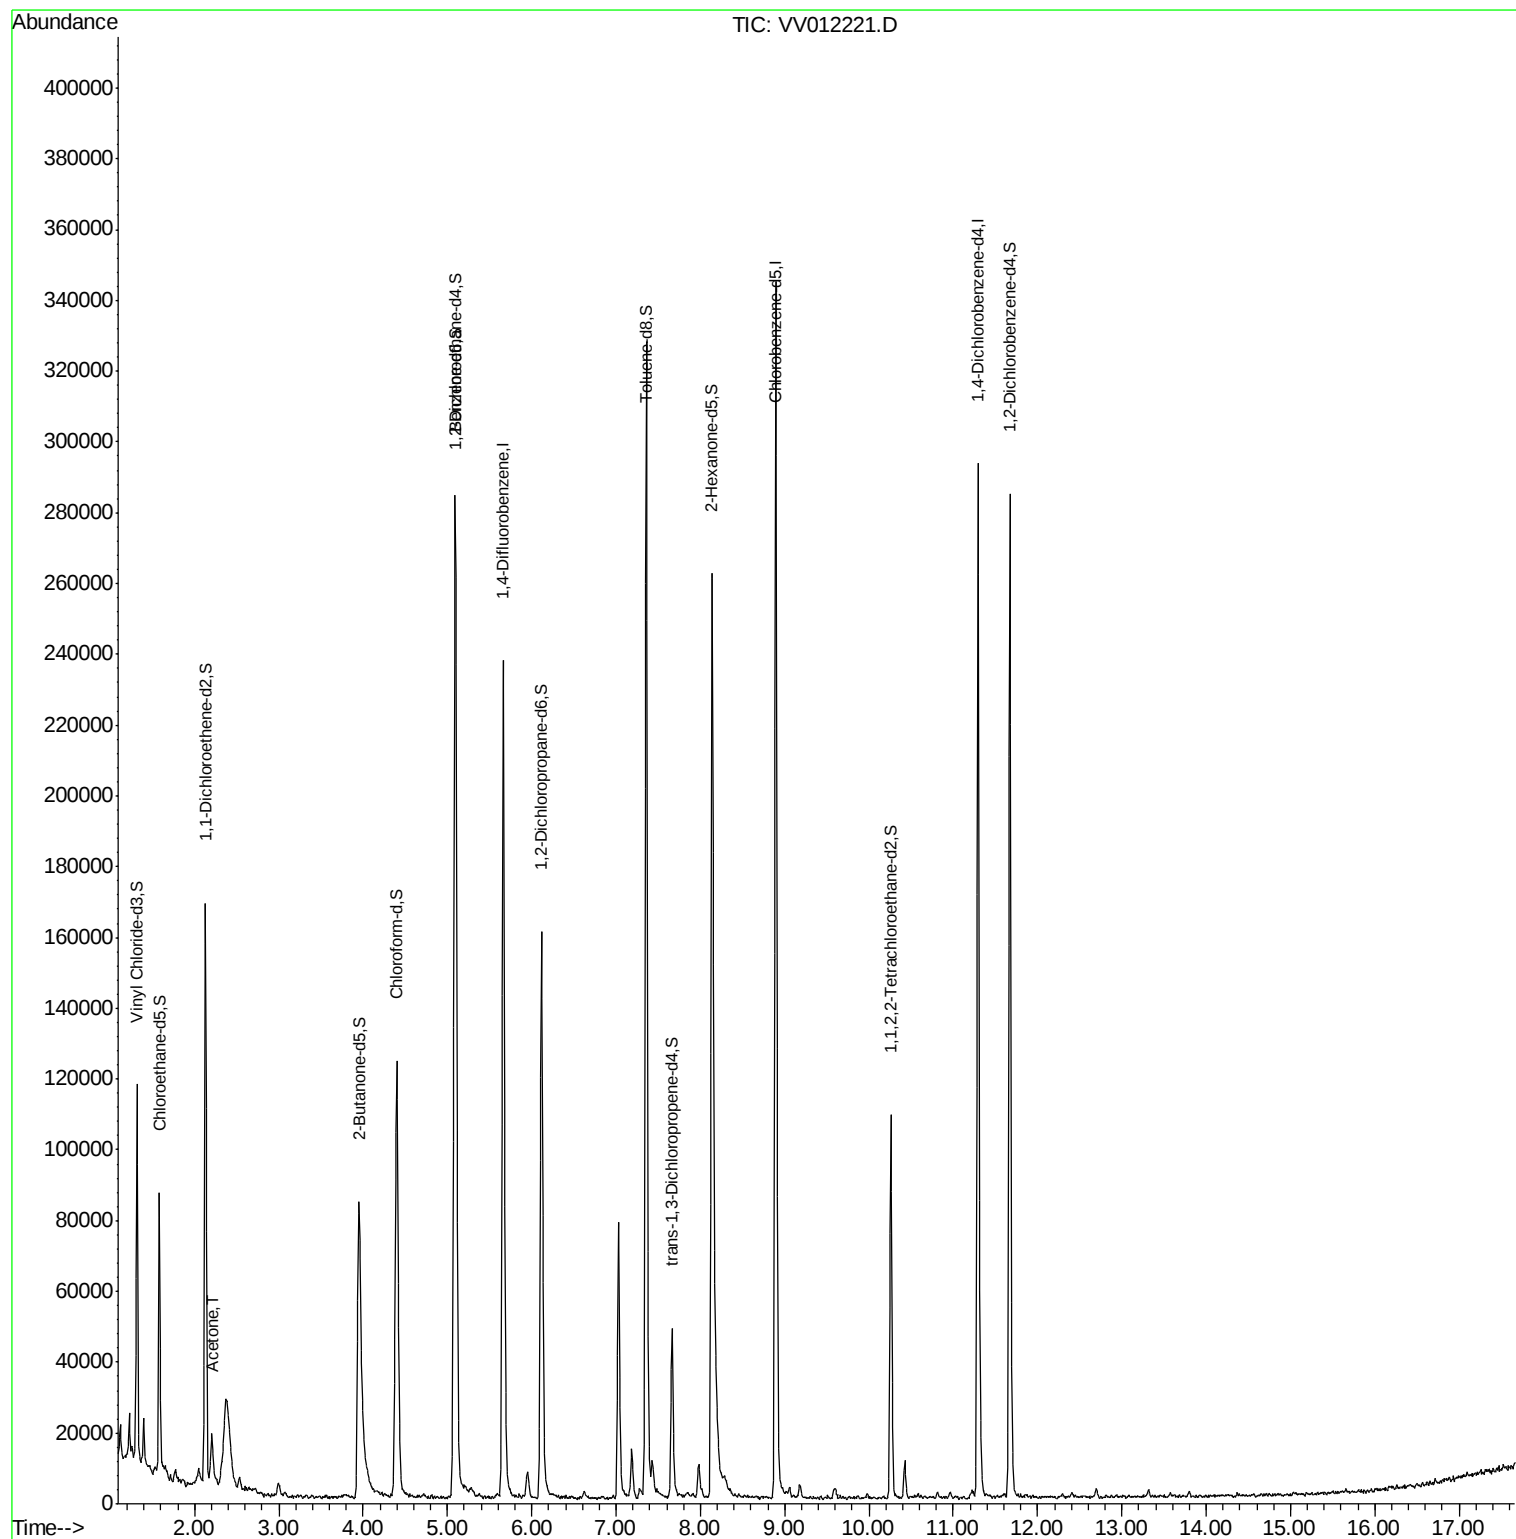

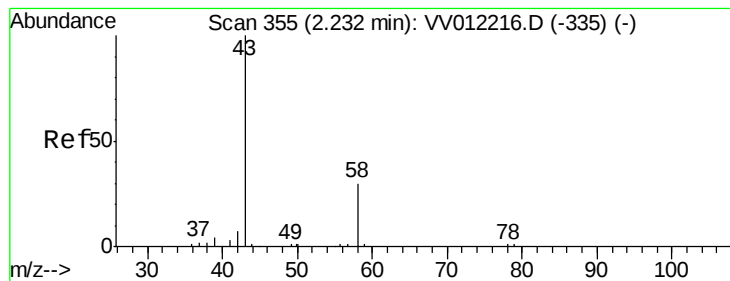

#13

Acetone

Concen: 11.018 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.03 min

Lab File: VV012221.D

Acq: 13 Aug 2019 18:12

Instrument :
MSVOA_V
ClientSampleId :
C0AJ2

Tgt Ion: 43 Resp: 18157

Ion Ratio Lower Upper

43 100

58 33.2 0.0 59.4

