

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
 Data File : VV012222.D
 Acq On : 13 Aug 2019 18:40
 Operator : SY/MD
 Sample : K4337-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG2

Quant Time: Aug 14 04:02:27 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 14 02:48:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	212432	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	205012	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	86980	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	58574	4.47	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.40%
7) Chloroethane-d5	1.58	69	48298	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.60%
11) 1,1-Dichloroethene-d2	2.13	63	74352	3.47	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.40%
20) 2-Butanone-d5	3.95	46	17083	6.04	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	12.08%#
24) Chloroform-d	4.40	84	106741	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.40%
26) 1,2-Dichloroethane-d4	5.08	65	59415	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.10	84	240570	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.80%
36) 1,2-Dichloropropane-d6	6.12	67	72274	4.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.60%
41) Toluene-d8	7.36	98	206877	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.40%
43) trans-1,3-Dichloropropene-	7.66	79	25470	4.35	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.00%
46) 2-Hexanone-d5	8.13	63	40947	21.82	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	43.64%#
57) 1,1,2,2-Tetrachloroethane-	10.26	84	44569	4.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	74422	5.06	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.20%


Target Compounds					Qvalue
13) Acetone	2.18	43	28283	16.056 ug/L	97
21) 2-Butanone	4.01	43	59856	16.618 ug/L	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
Data File : VV012222.D
Acq On : 13 Aug 2019 18:40
Operator : SY/MD
Sample : K4337-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG2

Quant Time: Aug 14 04:02:27 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 14 02:48:55 2019
Response via : Initial Calibration

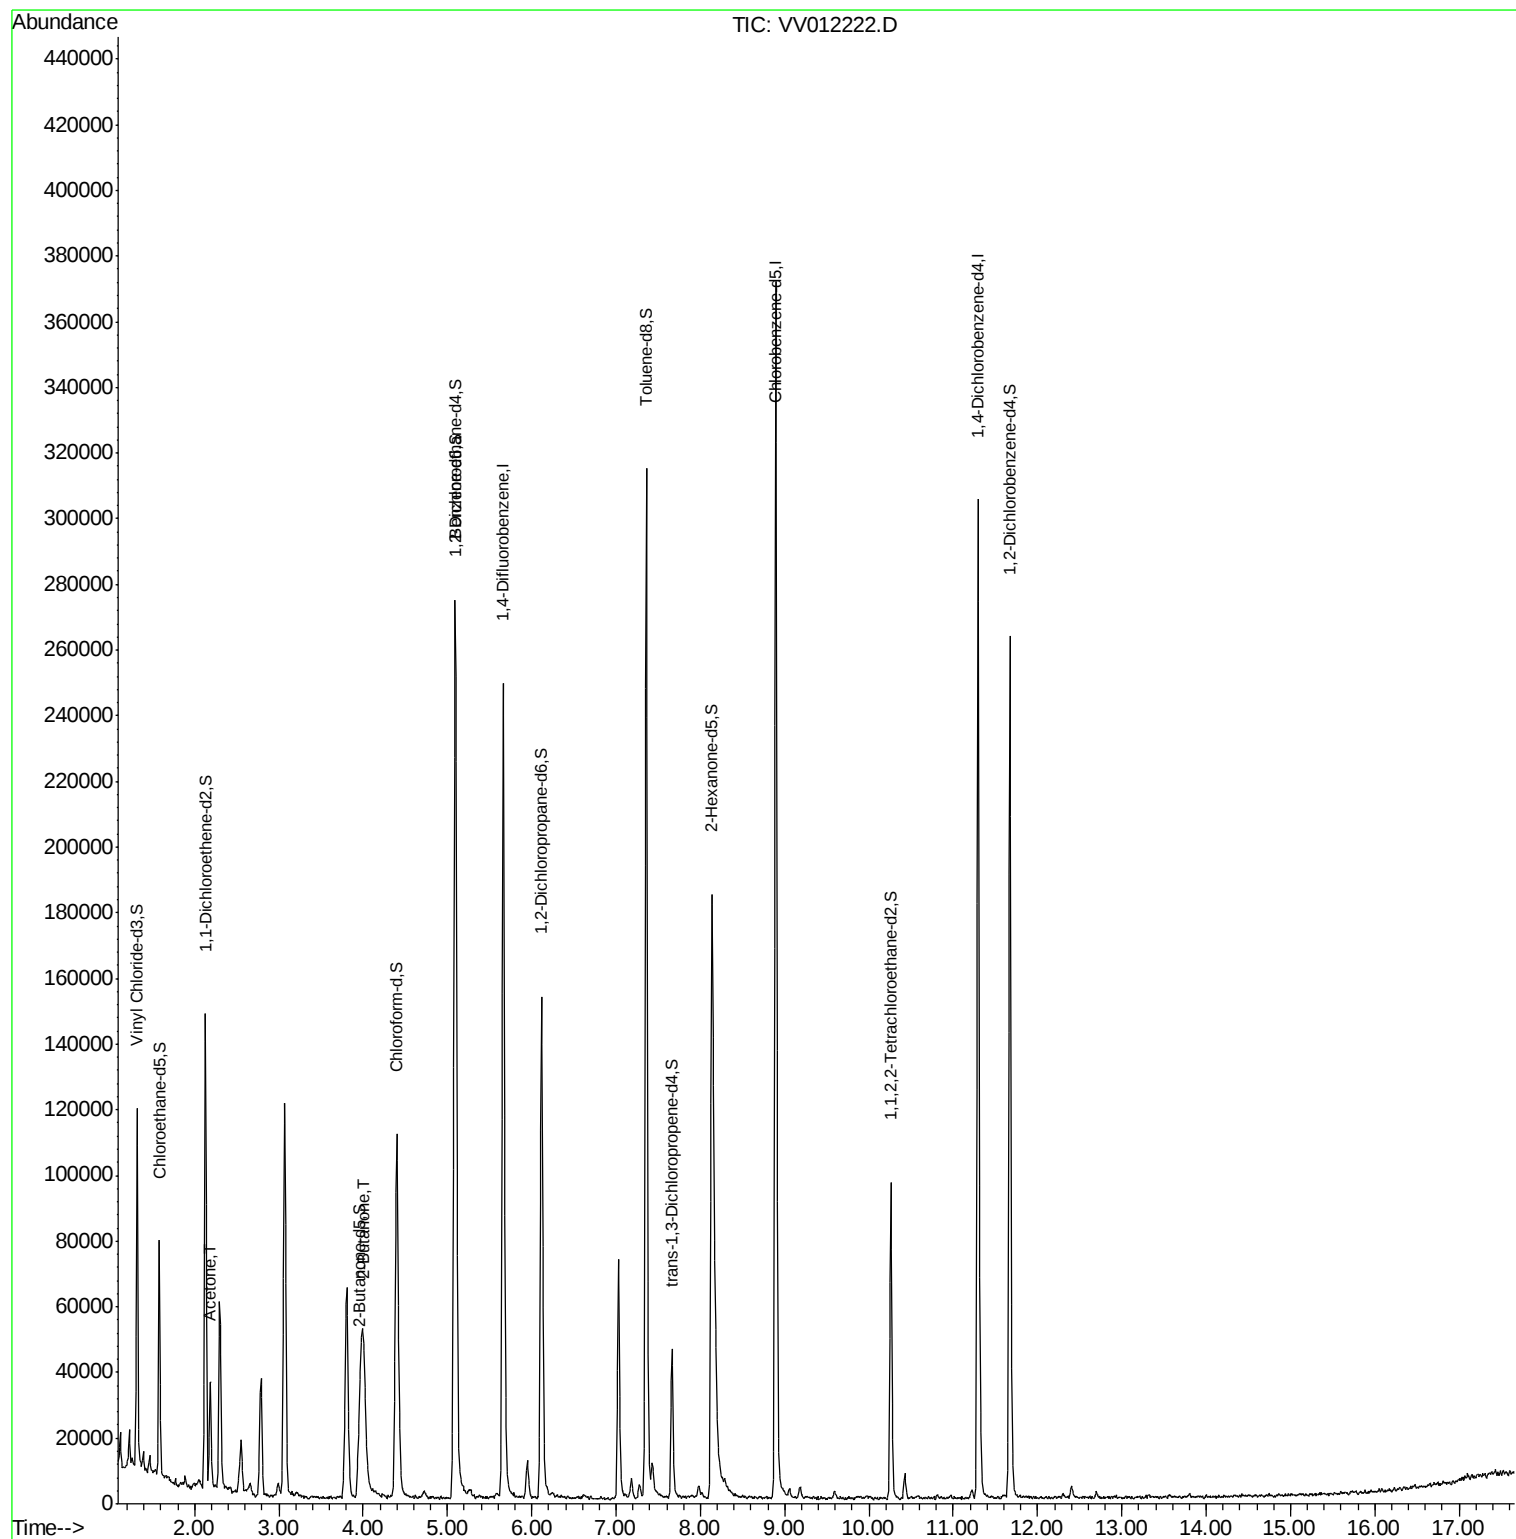

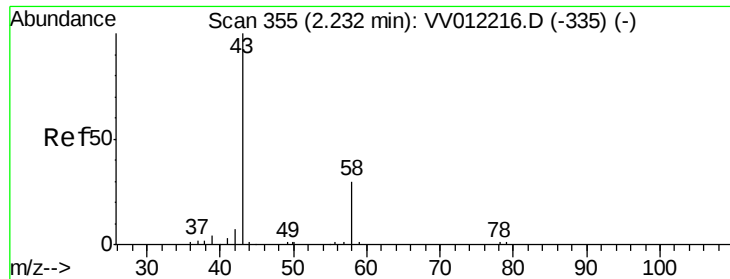

#13

Acetone

Concen: 16.056 ug/L

RT: 2.18 min Scan# 340

Delta R.T. -0.05 min

Lab File: VV012222.D

Acq: 13 Aug 2019 18:40

Instrument :

MSVOA_V

ClientSampleId :


C0AG2

Tgt Ion: 43 Resp: 28283

Ion Ratio Lower Upper

43 100

58 31.4 0.0 59.4

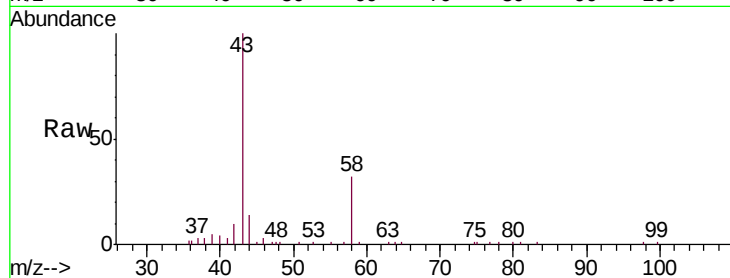

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

20000

15000

10000

5000

0



2.18

2.15

2.20

2.25

Time-->

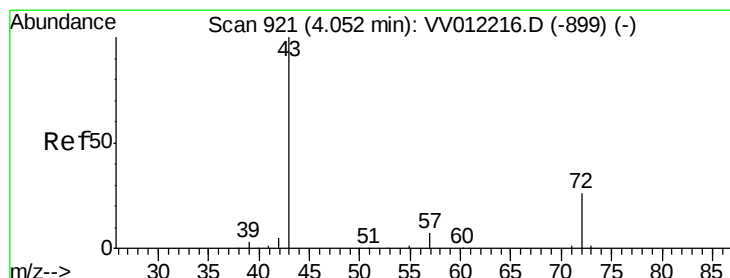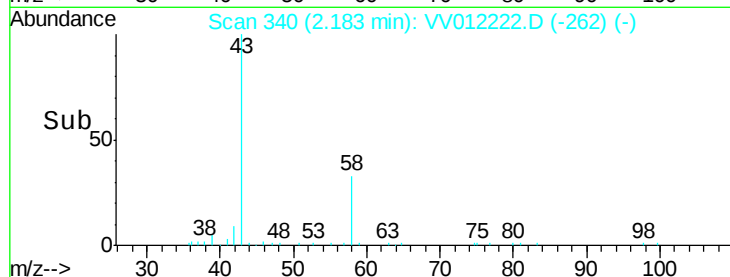

#21

2-Butanone

Concen: 16.618 ug/L

RT: 4.01 min Scan# 909

Delta R.T. -0.04 min

Lab File: VV012222.D


Acq: 13 Aug 2019 18:40

Tgt Ion: 43 Resp: 59856

Ion Ratio Lower Upper

43 100

72 13.5 12.9 38.7

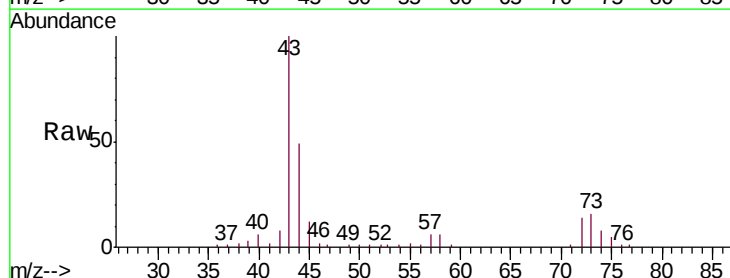

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 72.10 (71.80 to 72.80): VV0

20000

15000

10000

5000

0

4.01

3.90

4.10

Time-->

