

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
 Data File : VV012224.D
 Acq On : 13 Aug 2019 19:35
 Operator : SY/MD
 Sample : K4337-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC6

Quant Time: Aug 14 04:08:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 14 02:48:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	202415	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	196475	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	83710	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	57296	4.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.80%
7) Chloroethane-d5	1.58	69	46145	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.80%
11) 1,1-Dichloroethene-d2	2.13	63	72984	3.57	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.40%
20) 2-Butanone-d5	3.94	46	144622	53.70	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.40%
24) Chloroform-d	4.40	84	114825	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.00%
26) 1,2-Dichloroethane-d4	5.08	65	57577	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.60%
32) Benzene-d6	5.10	84	235212	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
36) 1,2-Dichloropropane-d6	6.12	67	70294	4.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.00%
41) Toluene-d8	7.36	98	198025	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.20%
43) trans-1,3-Dichloropropene-	7.66	79	24992	4.46	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.20%
46) 2-Hexanone-d5	8.14	63	90631	50.39	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.78%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	49187	4.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	71903	5.07	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.40%


Target Compounds					Qvalue
13) Acetone	2.19	43	3985	2.374 ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
Data File : VV012224.D
Acq On : 13 Aug 2019 19:35
Operator : SY/MD
Sample : K4337-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC6

Quant Time: Aug 14 04:08:35 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 14 02:48:55 2019
Response via : Initial Calibration

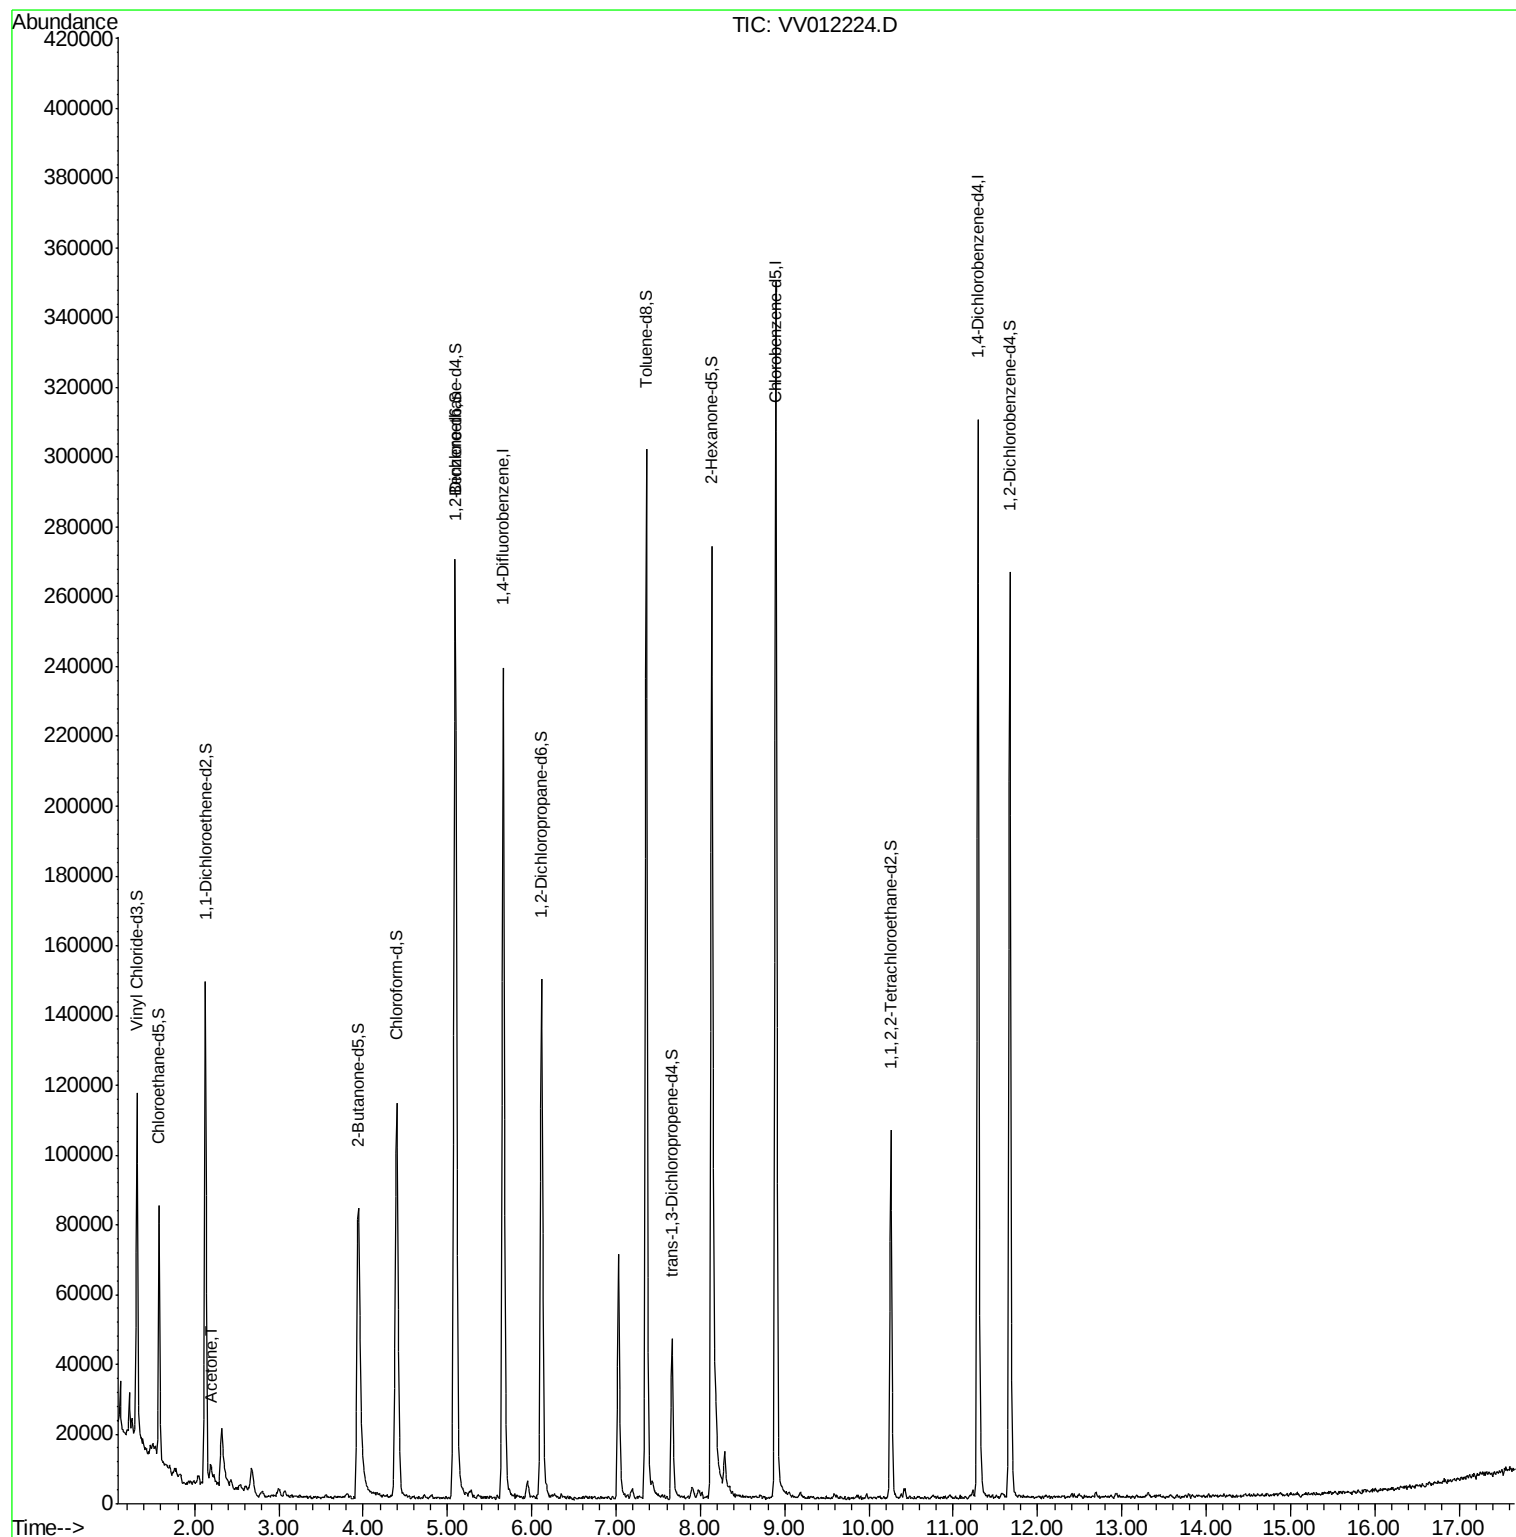

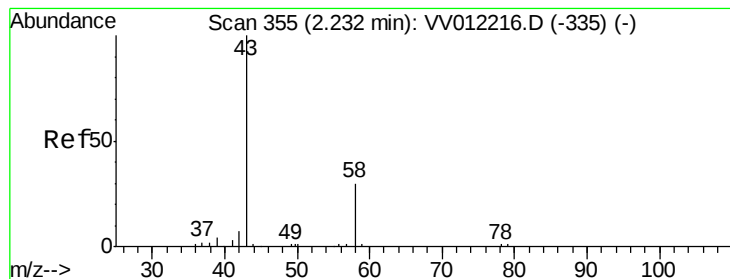

#13

Acetone

Concen: 2.374 ug/L

RT: 2.19 min Scan# 343

Delta R.T. -0.04 min

Lab File: VV012224.D

Acq: 13 Aug 2019 19:35

Instrument :
MSVOA_V
ClientSampleId :
C0AC6

Tgt Ion: 43 Resp: 3985

Ion Ratio Lower Upper

43 100

58 37.0 0.0 59.4

