

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
 Data File : VV012227.D
 Acq On : 13 Aug 2019 20:58
 Operator : SY/MD
 Sample : K4337-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE6

Quant Time: Aug 14 04:17:53 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 14 02:48:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	190946	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	187574	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	78670	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	58219	4.95	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.00%
7) Chloroethane-d5	1.58	69	47329	5.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.20%
11) 1,1-Dichloroethene-d2	2.13	63	78973	4.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.00%
20) 2-Butanone-d5	3.93	46	148878	58.60	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.20%
24) Chloroform-d	4.40	84	118325	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
26) 1,2-Dichloroethane-d4	5.08	65	60898	5.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.40%
32) Benzene-d6	5.10	84	236766	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.80%
36) 1,2-Dichloropropane-d6	6.12	67	70930	5.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.40%
41) Toluene-d8	7.36	98	197026	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%
43) trans-1,3-Dichloropropene-	7.66	79	23912	4.47	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.40%
46) 2-Hexanone-d5	8.13	63	88826	51.73	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.46%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	51373	5.27	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	71786	5.39	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.80%


Target Compounds					Qvalue
13) Acetone	2.19	43	11268	7.117 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
Data File : VV012227.D
Acq On : 13 Aug 2019 20:58
Operator : SY/MD
Sample : K4337-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE6

Quant Time: Aug 14 04:17:53 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 14 02:48:55 2019
Response via : Initial Calibration

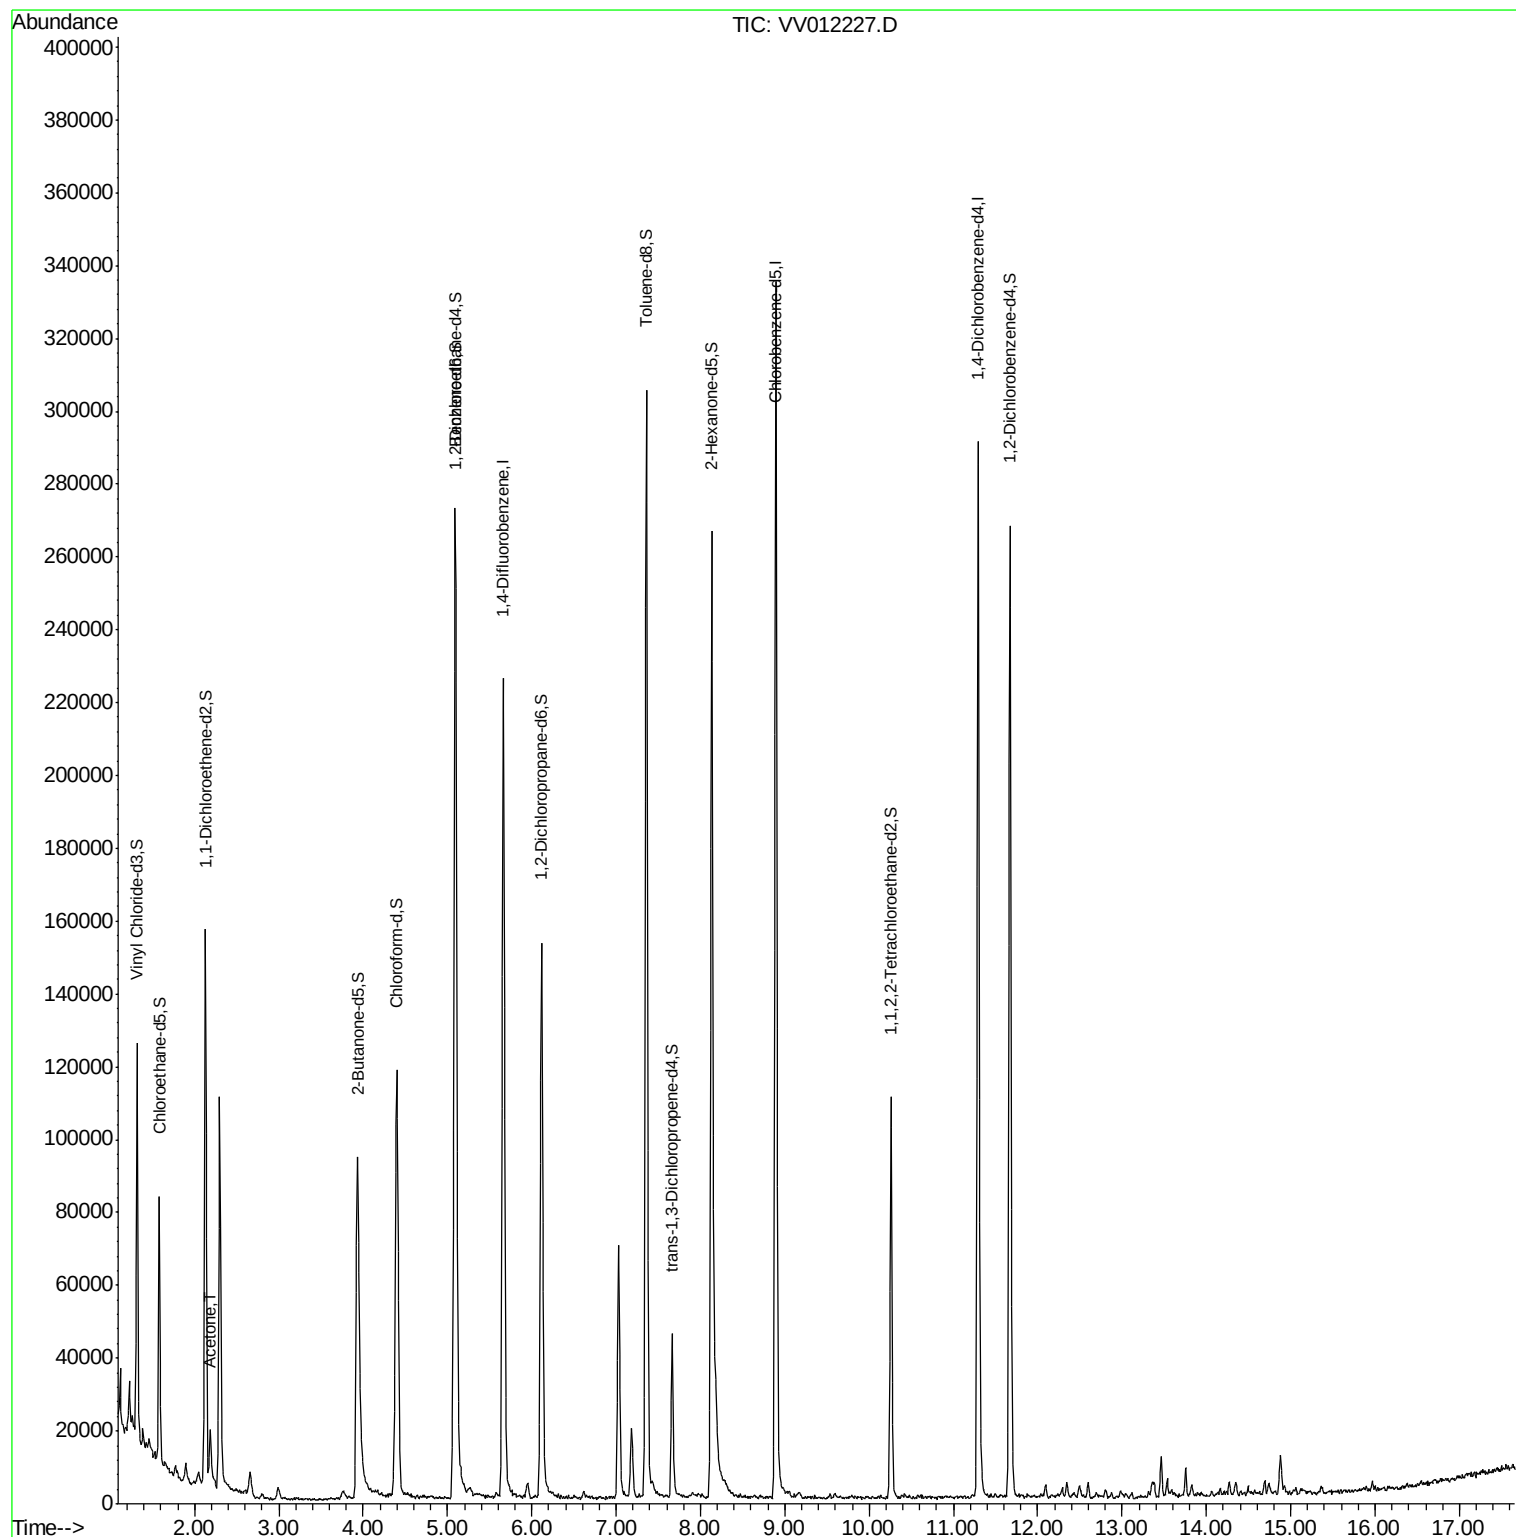

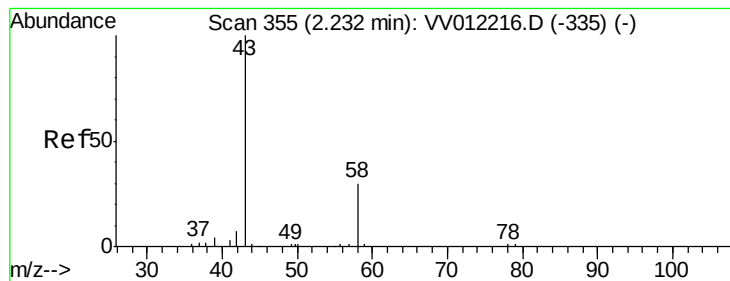

#13
 Acetone
 Concen: 7.117 ug/L
 RT: 2.19 min Scan# 341
 Delta R.T. -0.05 min
 Lab File: VV012227.D
 Acq: 13 Aug 2019 20:58

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE6

Tgt Ion: 43 Resp: 11268
 Ion Ratio Lower Upper
 43 100
 58 33.2 0.0 59.4

