

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
 Data File : VV012228.D
 Acq On : 13 Aug 2019 21:25
 Operator : SY/MD
 Sample : K4337-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE8

Quant Time: Aug 14 04:20:47 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 14 02:48:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	205877	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	199398	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	83186	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	56137	4.43	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.60%
7) Chloroethane-d5	1.58	69	47044	4.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.00%
11) 1,1-Dichloroethene-d2	2.13	63	73224	3.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.60%
20) 2-Butanone-d5	3.94	46	141345	51.60	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.20%
24) Chloroform-d	4.40	84	117488	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.60%
26) 1,2-Dichloroethane-d4	5.08	65	58840	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.00%
32) Benzene-d6	5.10	84	232561	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.20%
36) 1,2-Dichloropropane-d6	6.12	67	70376	4.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.60%
41) Toluene-d8	7.36	98	198513	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.20%
43) trans-1,3-Dichloropropene-	7.66	79	23345	4.10	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.00%
46) 2-Hexanone-d5	8.14	63	86547	47.41	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.82%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	50179	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	72409	5.14	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.80%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	2.20	43	3686	2.159	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081319\
Data File : VV012228.D
Acq On : 13 Aug 2019 21:25
Operator : SY/MD
Sample : K4337-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE8

Quant Time: Aug 14 04:20:47 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 14 02:48:55 2019
Response via : Initial Calibration

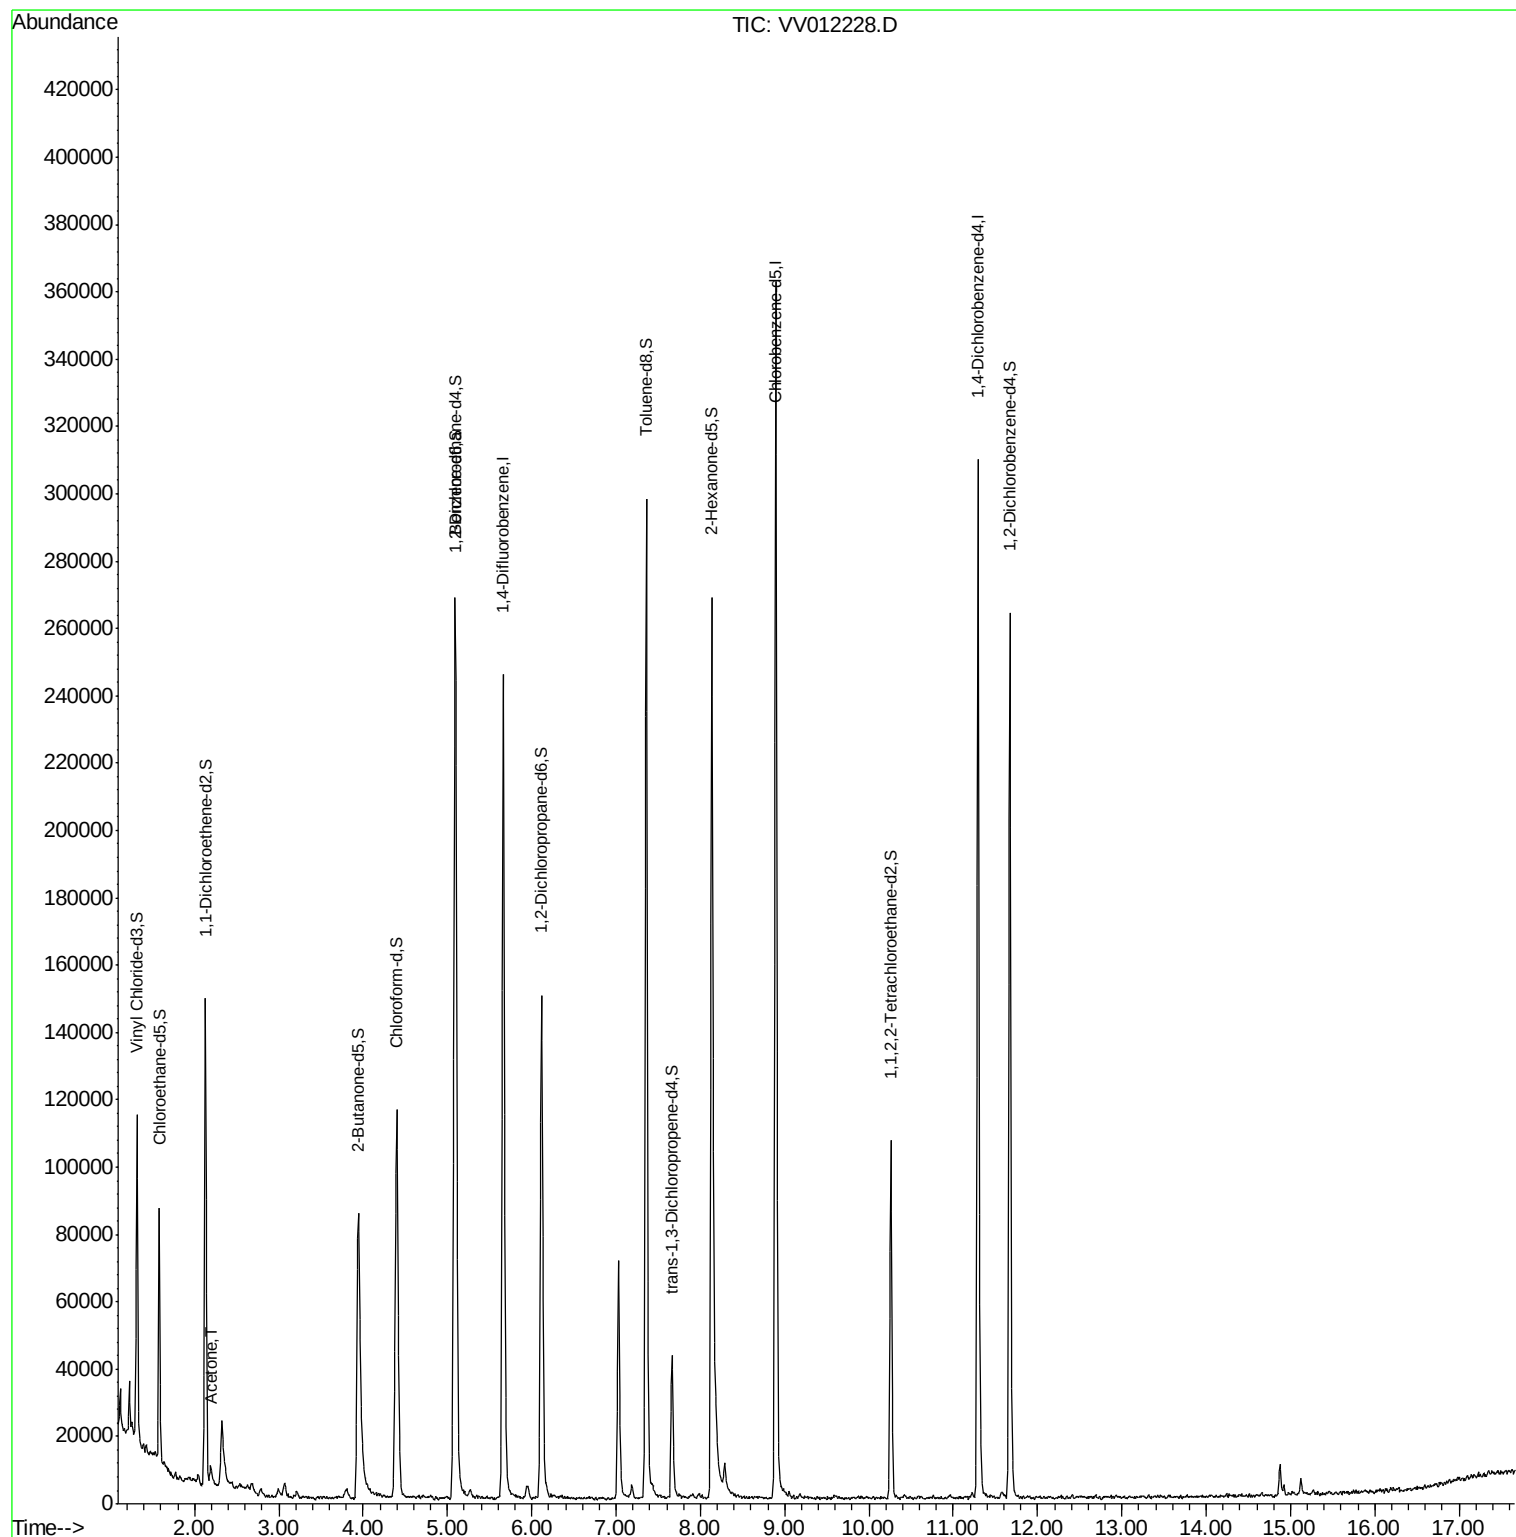

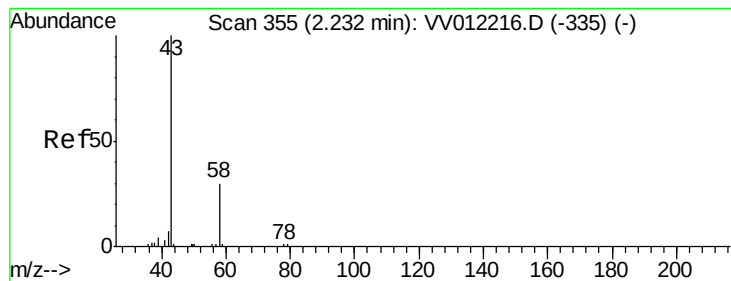

#13

Acetone

Concen: 2.159 ug/L

RT: 2.20 min Scan# 344

Delta R.T. -0.04 min

Lab File: VV012228.D

Acq: 13 Aug 2019 21:25

Instrument :
MSVOA_V
ClientSampleId :
C0AE8

Tgt Ion: 43 Resp: 3686

Ion Ratio Lower Upper

43 100

58 35.4 0.0 59.4

