


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV081319\
Data File : VV012213.D
Acq On : 13 Aug 2019 13:51
Operator : SY/MD
Sample : BFB46
Misc : 5mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB46

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Aug 14 02:48:55 2019

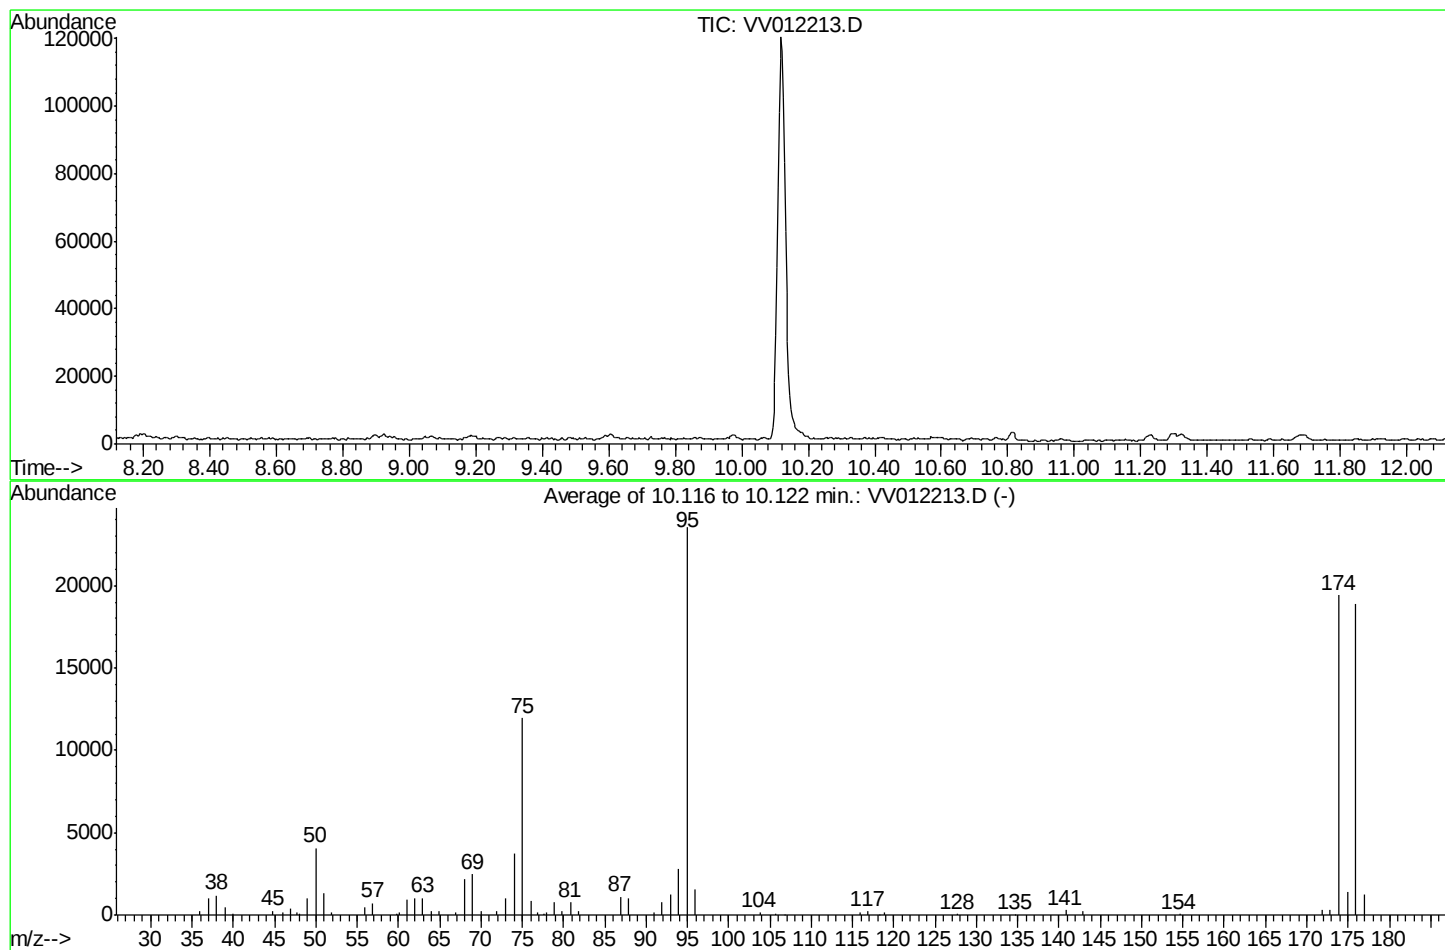

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	4059	PASS
75	95	30	80	50.8	11956	PASS
95	95	100	100	100.0	23541	PASS
96	95	5	9	6.7	1572	PASS
173	174	0.00	2	1.5	296	PASS
174	95	50	120	82.5	19410	PASS
175	174	5	9	7.4	1432	PASS
176	174	95	101	97.3	18890	PASS
177	176	5	9	6.6	1254	PASS

m/z	Abundance
35.80	244.0
37.00	1083.0
38.00	1178.0
39.00	413.0
39.90	793.0
43.80	571.0
44.80	310.0
46.00	121.0
47.00	350.0
47.70	197.0
48.00	195.0
48.90	991.0
50.00	3930.0
50.90	1291.0
51.90	164.0
55.90	452.0
56.90	712.0
60.10	193.0
61.00	930.0
62.00	970.0
62.90	955.0
64.00	190.0
65.00	204.0
67.00	150.0
67.90	2256.0
68.90	2498.0
70.00	166.0
71.80	201.0
73.00	973.0
74.00	3596.0
75.00	11871.0
76.00	884.0
76.80	150.0
78.00	137.0
78.80	760.0
79.70	242.0
80.80	739.0
81.90	182.0
86.90	1197.0
87.90	967.0
90.90	149.0
91.90	769.0
92.90	1245.0
93.90	2777.0
95.00	22832.0
95.90	1633.0
103.80	145.0
106.80	107.0
115.80	109.0
116.90	219.0
118.20	111.0
118.90	129.0
140.80	274.0
142.90	274.0
171.80	281.0
172.80	282.0
173.90	18720.0
174.90	1375.0
175.90	18128.0
176.90	1198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
35.80	204.0
36.90	1043.0
38.00	1241.0
39.00	451.0
39.90	804.0
43.90	543.0
44.80	272.0
46.00	134.0
46.90	380.0
47.70	195.0
48.90	1021.0
50.00	4166.0
50.90	1374.0
52.00	180.0
55.90	472.0
56.90	744.0
60.20	180.0
61.00	959.0
62.00	1022.0
62.90	1067.0
63.90	202.0
64.90	223.0
66.90	127.0
67.90	2267.0
69.00	2511.0
70.00	232.0
71.90	219.0
73.00	1026.0
74.00	3782.0
75.00	12405.0
76.00	863.0
76.90	190.0
77.60	133.0
77.90	143.0
78.80	768.0
79.80	270.0
80.80	751.0
81.80	209.0
86.90	1169.0
87.90	1009.0
90.90	179.0
91.90	814.0
93.00	1299.0
93.90	2859.0
95.00	24384.0
95.90	1624.0
103.80	130.0
105.60	116.0
115.90	128.0
116.90	235.0
118.90	151.0
127.70	109.0
140.80	311.0
142.90	264.0
154.60	109.0
171.80	308.0
172.70	306.0
173.90	19928.0
174.90	1448.0
175.90	19544.0
176.90	1282.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
35.90	214.0
36.90	1003.0
38.00	1153.0
38.90	448.0
39.90	806.0
43.90	632.0
44.80	214.0
46.10	123.0
46.90	373.0
47.80	174.0
48.90	1105.0
50.00	4083.0
50.90	1391.0
52.00	132.0
55.90	429.0
56.90	673.0
59.80	172.0
61.00	941.0
62.00	1093.0
63.00	1090.0
63.80	230.0
64.90	223.0
66.80	107.0
68.00	2087.0
69.00	2356.0
70.00	287.0
71.90	208.0
73.00	983.0
74.00	3726.0
75.00	11594.0
76.00	819.0
76.90	198.0
78.00	143.0
78.80	761.0
79.90	293.0
80.90	744.0
81.80	208.0
86.90	976.0
87.90	981.0
90.90	166.0
91.90	748.0
93.00	1196.0
93.90	2721.0
95.00	23408.0
95.90	1461.0
103.80	101.0
105.60	132.0
115.90	130.0
116.90	197.0
118.90	155.0
127.80	119.0
134.70	112.0
140.80	293.0
142.80	280.0
154.60	115.0
171.90	333.0
172.70	301.0
173.90	19584.0
174.90	1473.0
175.90	19000.0
176.90	1283.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

Scan 2795 (10.077 min): VV012213.D
BFB46

m/z	Abundance
35.30	118.0
39.90	710.0
43.90	653.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46