


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV081320\
 Data File : VV017960.D
 Acq On : 13 Aug 2020 09:27
 Operator : SY/MD
 Sample : BFB73
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB73

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis
 Last Update : Fri Aug 14 04:14:46 2020

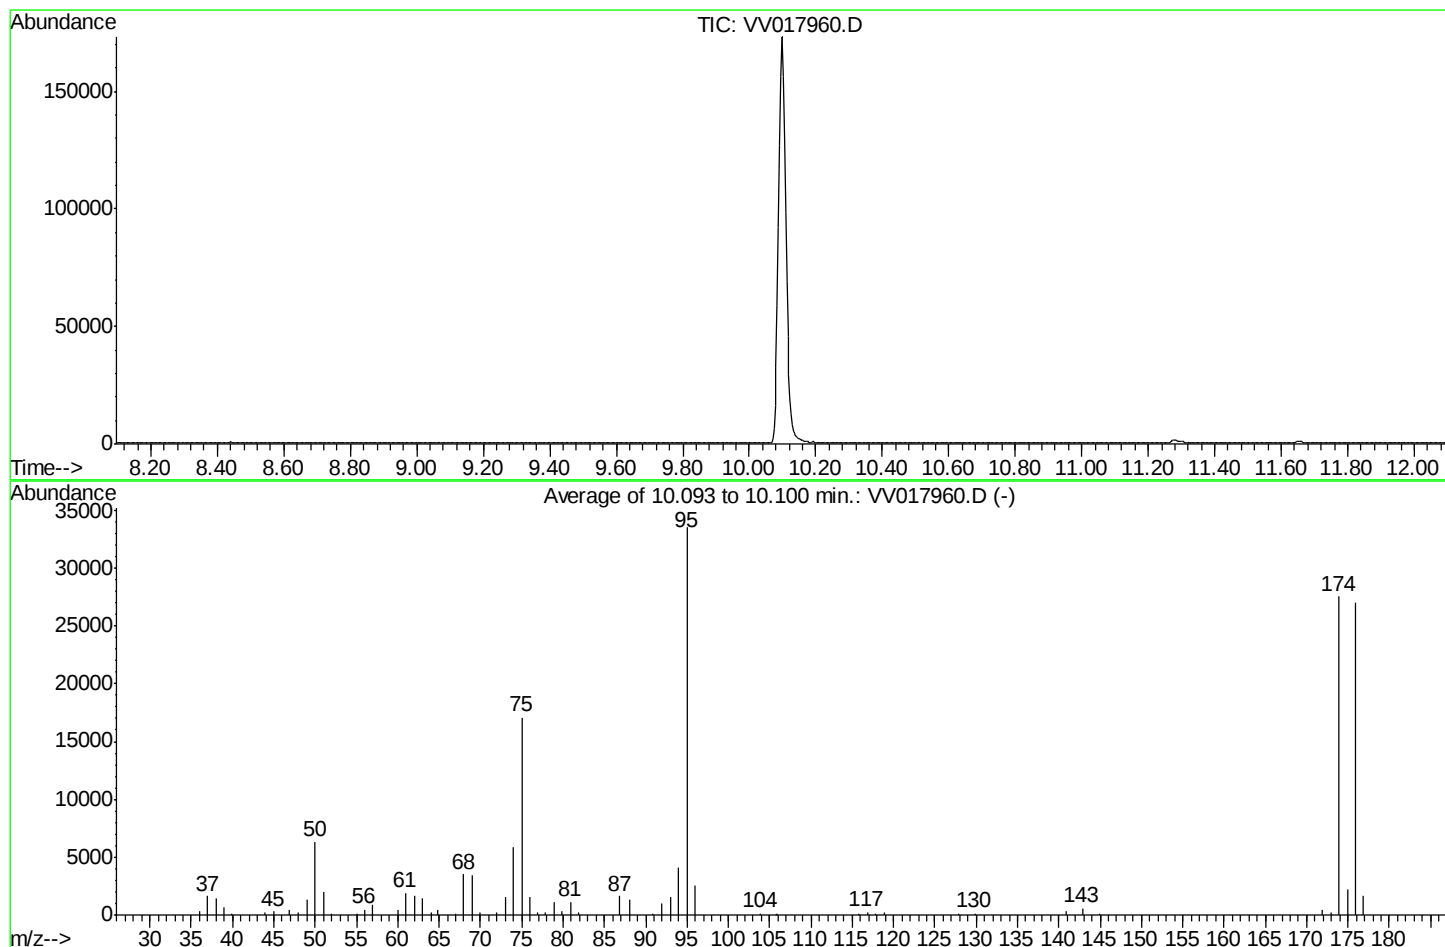

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	6358	PASS
75	95	30	80	51.0	17099	PASS
95	95	100	100	100.0	33525	PASS
96	95	5	9	7.5	2502	PASS
173	174	0.00	2	1.0	278	PASS
174	95	50	120	82.2	27546	PASS
175	174	5	9	7.9	2186	PASS
176	174	95	101	98.1	27016	PASS
177	176	5	9	6.2	1665	PASS

m/z	Abundance
35.90	322.0
37.00	1605.0
38.00	1449.0
39.00	668.0
39.90	210.0
43.90	427.0
45.00	246.0
46.90	436.0
47.90	273.0
49.00	1237.0
50.00	6162.0
51.00	1808.0
51.90	115.0
56.00	493.0
57.00	835.0
60.00	374.0
61.00	1761.0
62.00	1664.0
63.00	1331.0
64.00	263.0
64.90	522.0
67.00	122.0
68.00	3414.0
69.00	3351.0
70.00	286.0
71.90	181.0
73.00	1650.0
74.00	5579.0
75.00	15922.0
76.00	1494.0
76.90	253.0
77.80	193.0
78.90	1103.0
79.80	333.0
80.90	1073.0
81.90	232.0
86.90	1576.0
88.00	1250.0
90.90	141.0
92.00	950.0
93.00	1475.0
94.00	3886.0
95.00	31464.0
96.00	2454.0
103.90	125.0
105.70	114.0
115.80	102.0
116.80	290.0
117.80	152.0
118.80	208.0
129.90	102.0
140.90	297.0
142.90	527.0
144.90	177.0
171.90	452.0
173.90	25080.0
174.90	2024.0
175.90	24704.0
176.90	1536.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
35.90	323.0
37.00	1680.0
38.00	1555.0
39.00	729.0
39.90	223.0
43.90	477.0
45.00	310.0
46.90	466.0
47.90	260.0
49.00	1391.0
50.00	6499.0
51.00	2033.0
52.00	114.0
55.00	116.0
56.00	464.0
57.00	942.0
60.00	423.0
61.00	1978.0
62.00	1756.0
63.00	1423.0
64.00	282.0
64.90	501.0
67.00	125.0
68.00	3646.0
69.00	3532.0
70.00	269.0
71.90	222.0
73.00	1638.0
74.00	6044.0
75.00	17768.0
76.00	1644.0
76.90	221.0
77.90	204.0
78.90	1199.0
79.90	354.0
80.90	1175.0
81.90	248.0
86.90	1724.0
88.00	1411.0
90.80	135.0
92.00	987.0
92.90	1641.0
94.00	4261.0
95.00	34608.0
96.00	2593.0
103.90	140.0
105.90	139.0
115.90	133.0
116.80	290.0
117.80	170.0
118.90	249.0
128.00	113.0
129.90	120.0
140.90	354.0
142.90	586.0
144.90	156.0
171.90	506.0
172.90	399.0
173.90	28448.0
174.90	2235.0
175.90	27888.0
176.90	1712.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
36.00	301.0
37.00	1609.0
38.00	1442.0
39.00	707.0
39.90	235.0
43.90	549.0
44.90	358.0
46.90	411.0
48.00	225.0
49.00	1434.0
50.00	6413.0
51.00	2081.0
52.00	101.0
55.00	143.0
55.90	443.0
57.00	997.0
60.00	435.0
60.90	1983.0
62.00	1685.0
63.00	1437.0
64.00	271.0
64.90	458.0
67.00	109.0
68.00	3496.0
69.00	3414.0
70.00	246.0
71.90	231.0
73.00	1519.0
74.00	5912.0
75.00	17608.0
76.00	1623.0
76.90	179.0
77.90	205.0
78.90	1161.0
79.90	355.0
80.90	1150.0
81.90	284.0
86.90	1592.0
88.00	1334.0
90.90	116.0
92.00	969.0
92.90	1604.0
94.00	4204.0
95.00	34504.0
96.00	2459.0
103.90	150.0
105.90	155.0
115.80	155.0
116.80	249.0
117.80	155.0
118.90	234.0
127.90	105.0
129.80	122.0
140.90	404.0
142.90	603.0
144.80	135.0
171.90	522.0
172.90	435.0
173.90	29112.0
174.90	2301.0
175.90	28456.0
176.90	1749.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

Scan 2790 (10.061 min): VV017960.D
BFB73

m/z	Abundance
39.90	156.0
43.90	308.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73