


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV081325\
Data File : VV038944.D
Acq On : 13 Aug 2025 08:58
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V081325W.M
Title : SW846 8260
Last Update : Thu Aug 14 02:40:30 2025

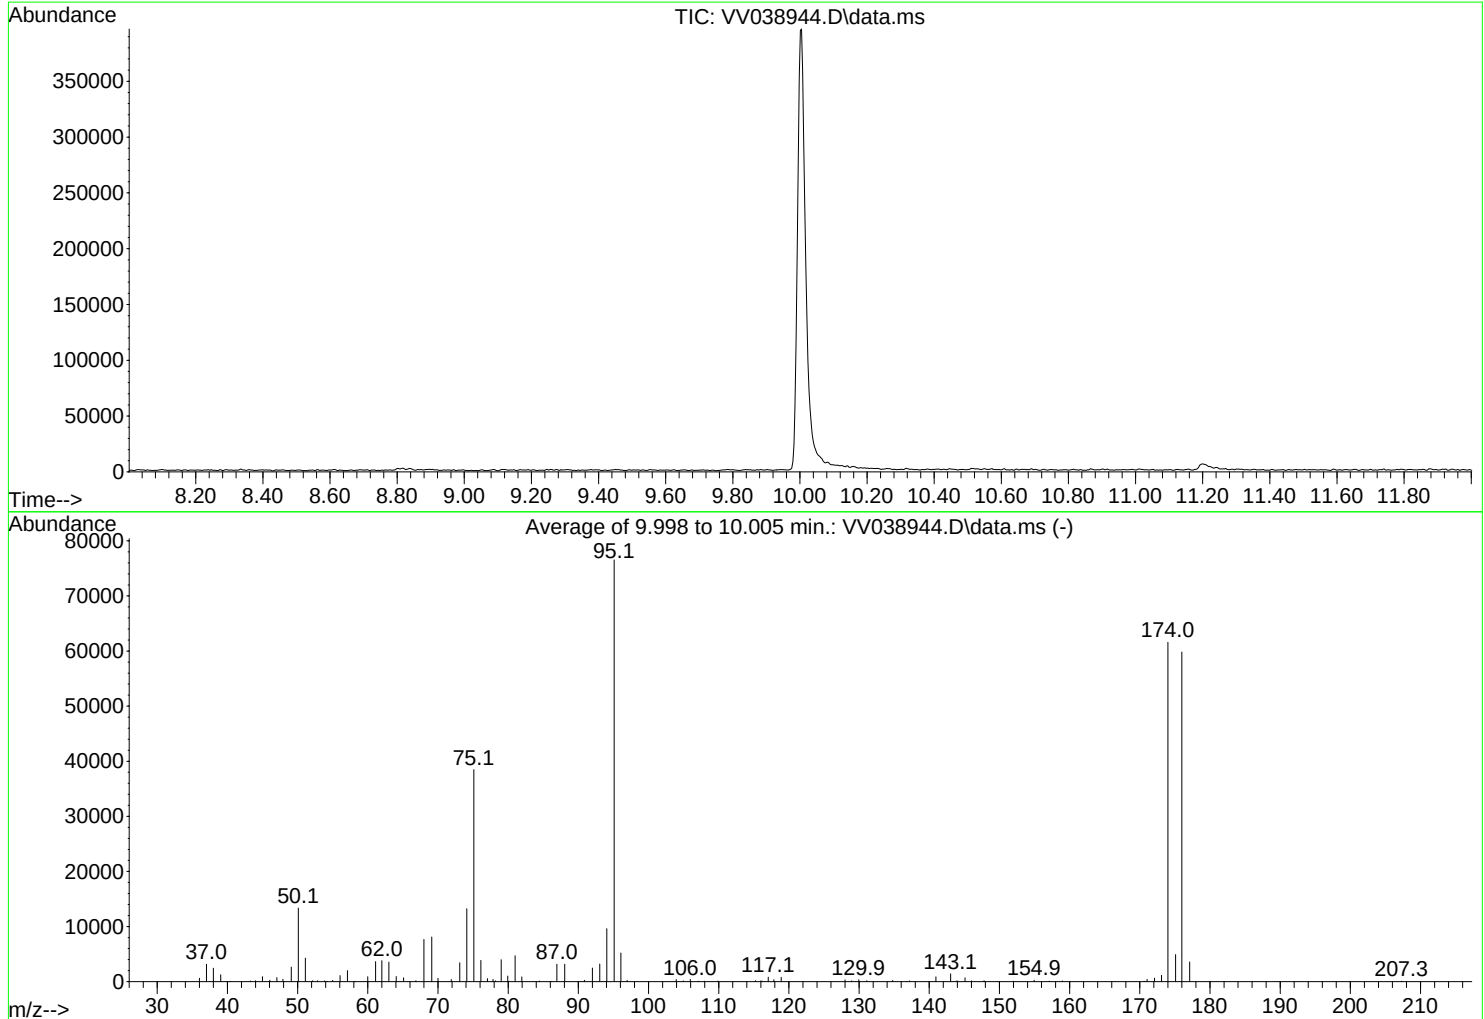

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2774

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	13362	PASS
75	95	30	60	50.3	38475	PASS
95	95	100	100	100.0	76555	PASS
96	95	5	9	6.8	5214	PASS
173	174	0.00	2	1.9	1157	PASS
174	95	50	100	80.5	61603	PASS
175	174	5	9	8.0	4920	PASS
176	174	95	101	97.1	59829	PASS
177	176	5	9	6.0	3566	PASS