




Data File : VV012244.D
Acq On : 14 Aug 2019 19:32
Operator : SY/MD
Sample : K4337-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ3

Manual Integrations
APPROVED

MMDadoda
8/16/2019 9:47:49 AM

Quant Time: Aug 15 23:33:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Aug 15 23:30:01 2019
Response via : Initial Calibration

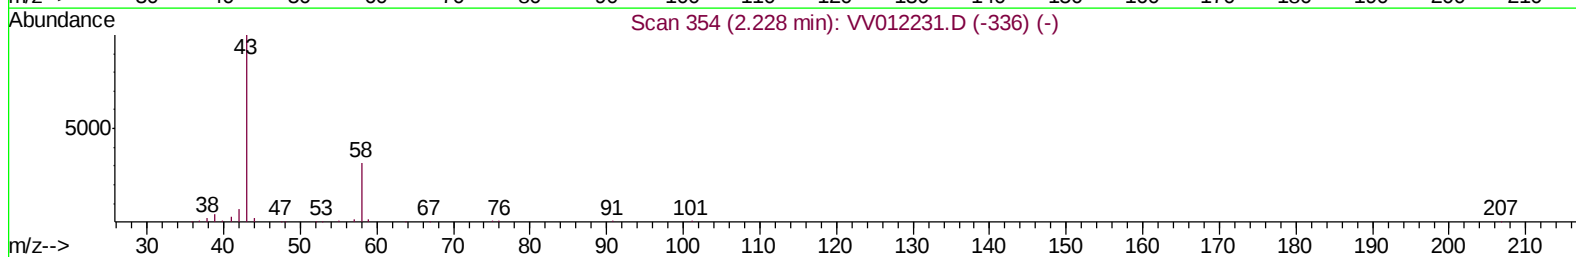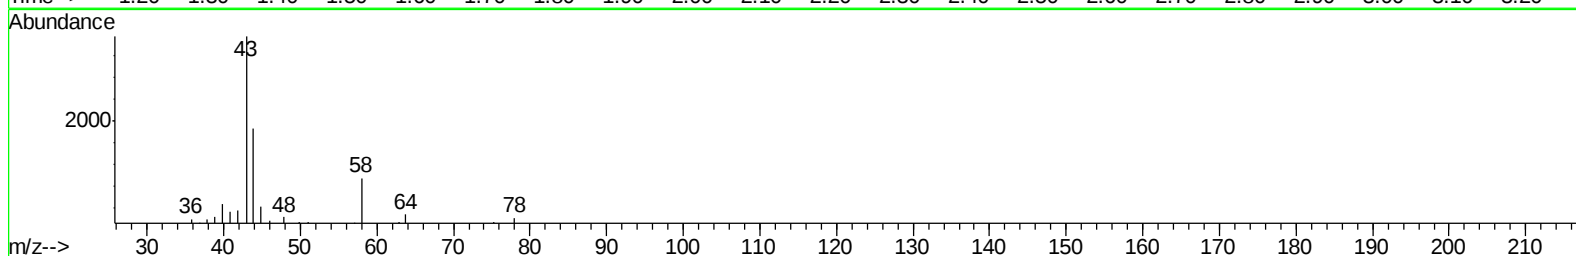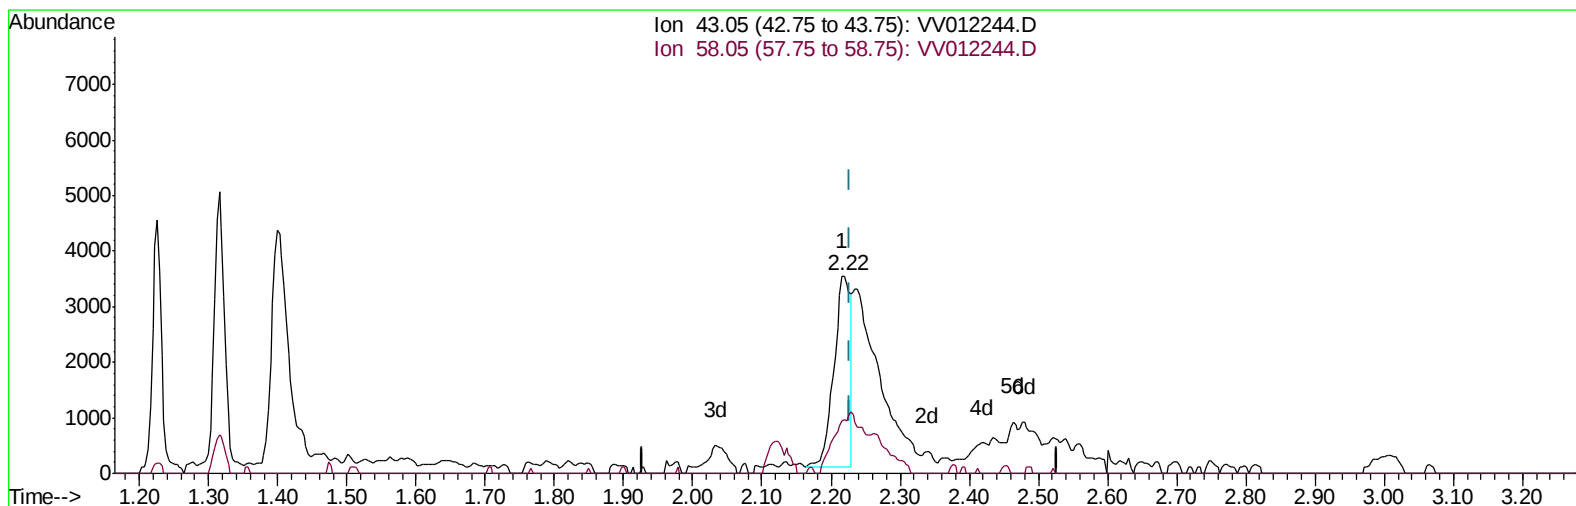

TIC: VV012244.D

(13) Acetone (T)

2.216min (-0.013) 3.76ug/L

response 5670

Ion	Exp%	Act%
43.05	100	100
58.05	29.70	55.34
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VV012244.D
Acq On : 14 Aug 2019 19:32
Operator : SY/MD
Sample : K4337-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ3

Manual Integrations
APPROVED

MMDadoda
8/16/2019 9:47:49 AM

Quant Time: Aug 15 23:33:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Aug 15 23:30:01 2019
Response via : Initial Calibration

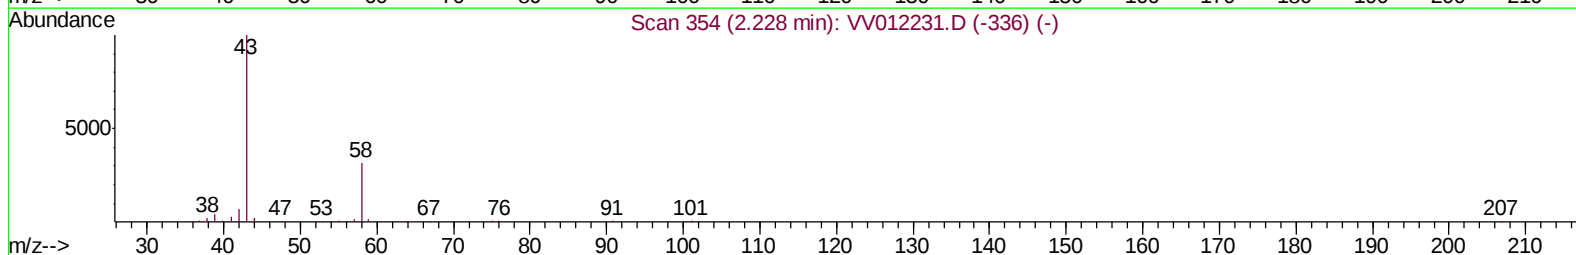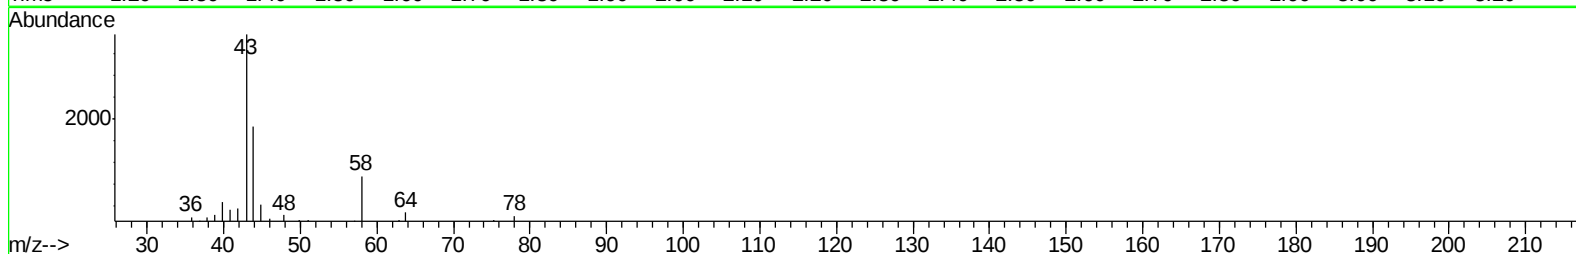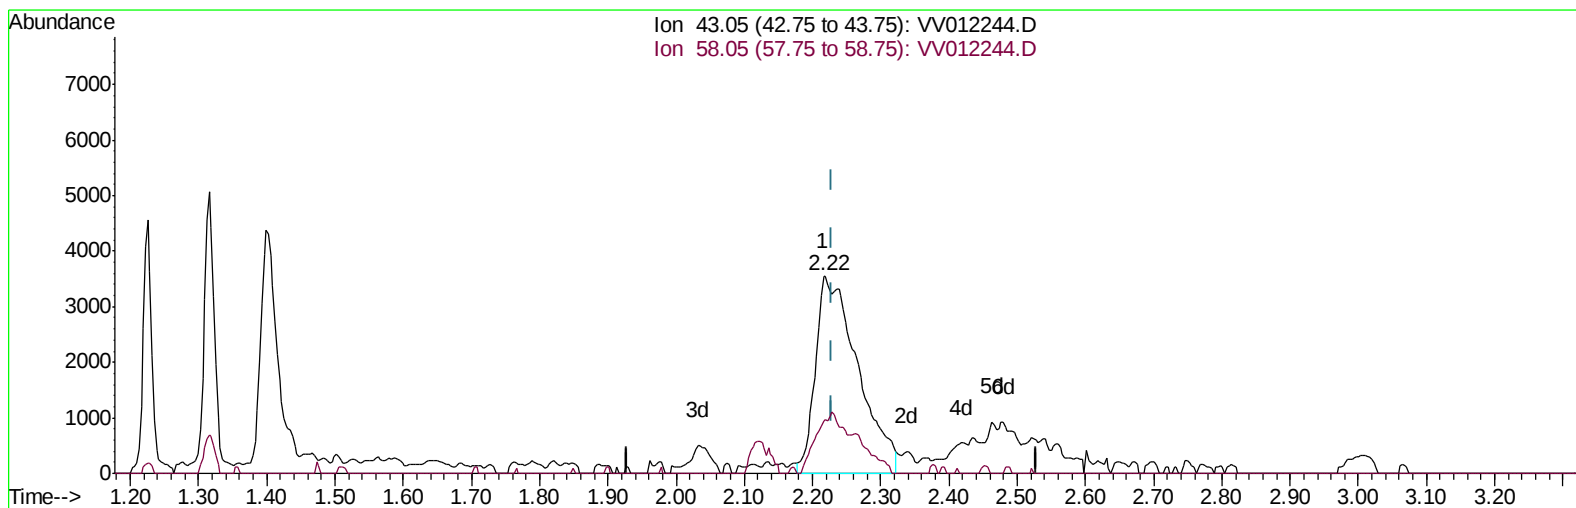

TIC: VV012244.D

(13) Acetone (T)

2.216min (-0.013) 10.13ug/L m

response 15285

Ion	Exp%	Act%
43.05	100	100
58.05	29.70	20.53
0.00	0.00	0.00
0.00	0.00	0.00

Data File : VV012244.D
Acq On : 14 Aug 2019 19:32
Operator : SY/MD
Sample : K4337-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ3

Manual Integrations
APPROVED

MMDadoda
8/16/2019 9:47:49 AM

Quant Time: Aug 16 00:15:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Aug 15 23:30:01 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	181941	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	178937	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	74531	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	51253	4.57	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.40%
7) Chloroethane-d5	1.58	69	44092	5.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.00%
11) 1,1-Dichloroethene-d2	2.13	63	62244	3.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.80%
20) 2-Butanone-d5	3.96	46	126147	52.11	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.22%
24) Chloroform-d	4.40	84	111731	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
26) 1,2-Dichloroethane-d4	5.08	65	57382	5.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.20%
32) Benzene-d6	5.10	84	221958	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
36) 1,2-Dichloropropane-d6	6.12	67	67480	5.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.20%
41) Toluene-d8	7.36	98	188961	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
43) trans-1,3-Dichloropropene-	7.67	79	24813	4.86	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.20%
46) 2-Hexanone-d5	8.14	63	80230	48.97	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.94%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	47070	5.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	67400	5.34	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.80%

Target Compounds					Qvalue
13) Acetone	2.22	43	15285m	10.131	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV012244.D
Acq On : 14 Aug 2019 19:32
Operator : SY/MD
Sample : K4337-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ3

Manual Integrations
APPROVED

MMDadoda
8/16/2019 9:47:49 AM

Quant Time: Aug 16 00:15:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Aug 15 23:30:01 2019
Response via : Initial Calibration

