

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081419\
 Data File : VV012236.D
 Acq On : 14 Aug 2019 15:52
 Operator : SY/MD
 Sample : K4337-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA0

Quant Time: Aug 15 19:17:59 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Aug 15 18:05:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	220973	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	216234	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	92331	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	53596	3.94	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.80%
7) Chloroethane-d5	1.58	69	44530	4.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.60%
11) 1,1-Dichloroethene-d2	2.13	63	71450	3.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.20%
20) 2-Butanone-d5	3.96	46	117034	39.80	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	79.60%
24) Chloroform-d	4.40	84	109385	4.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.20%
26) 1,2-Dichloroethane-d4	5.08	65	52504	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.40%
32) Benzene-d6	5.09	84	218863	4.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.00%
36) 1,2-Dichloropropane-d6	6.11	67	65012	4.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.60%
41) Toluene-d8	7.36	98	185185	3.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.20%
43) trans-1,3-Dichloropropene-	7.66	79	22790	3.69	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.80%
46) 2-Hexanone-d5	8.14	63	62660	31.65	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	63.30%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	41349	3.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	73.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	66210	4.24	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.80%


Target Compounds					Qvalue
13) Acetone	2.22	43	6455	3.523 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081419\
Data File : VV012236.D
Acq On : 14 Aug 2019 15:52
Operator : SY/MD
Sample : K4337-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA0

Quant Time: Aug 15 19:17:59 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Aug 15 18:05:57 2019
Response via : Initial Calibration

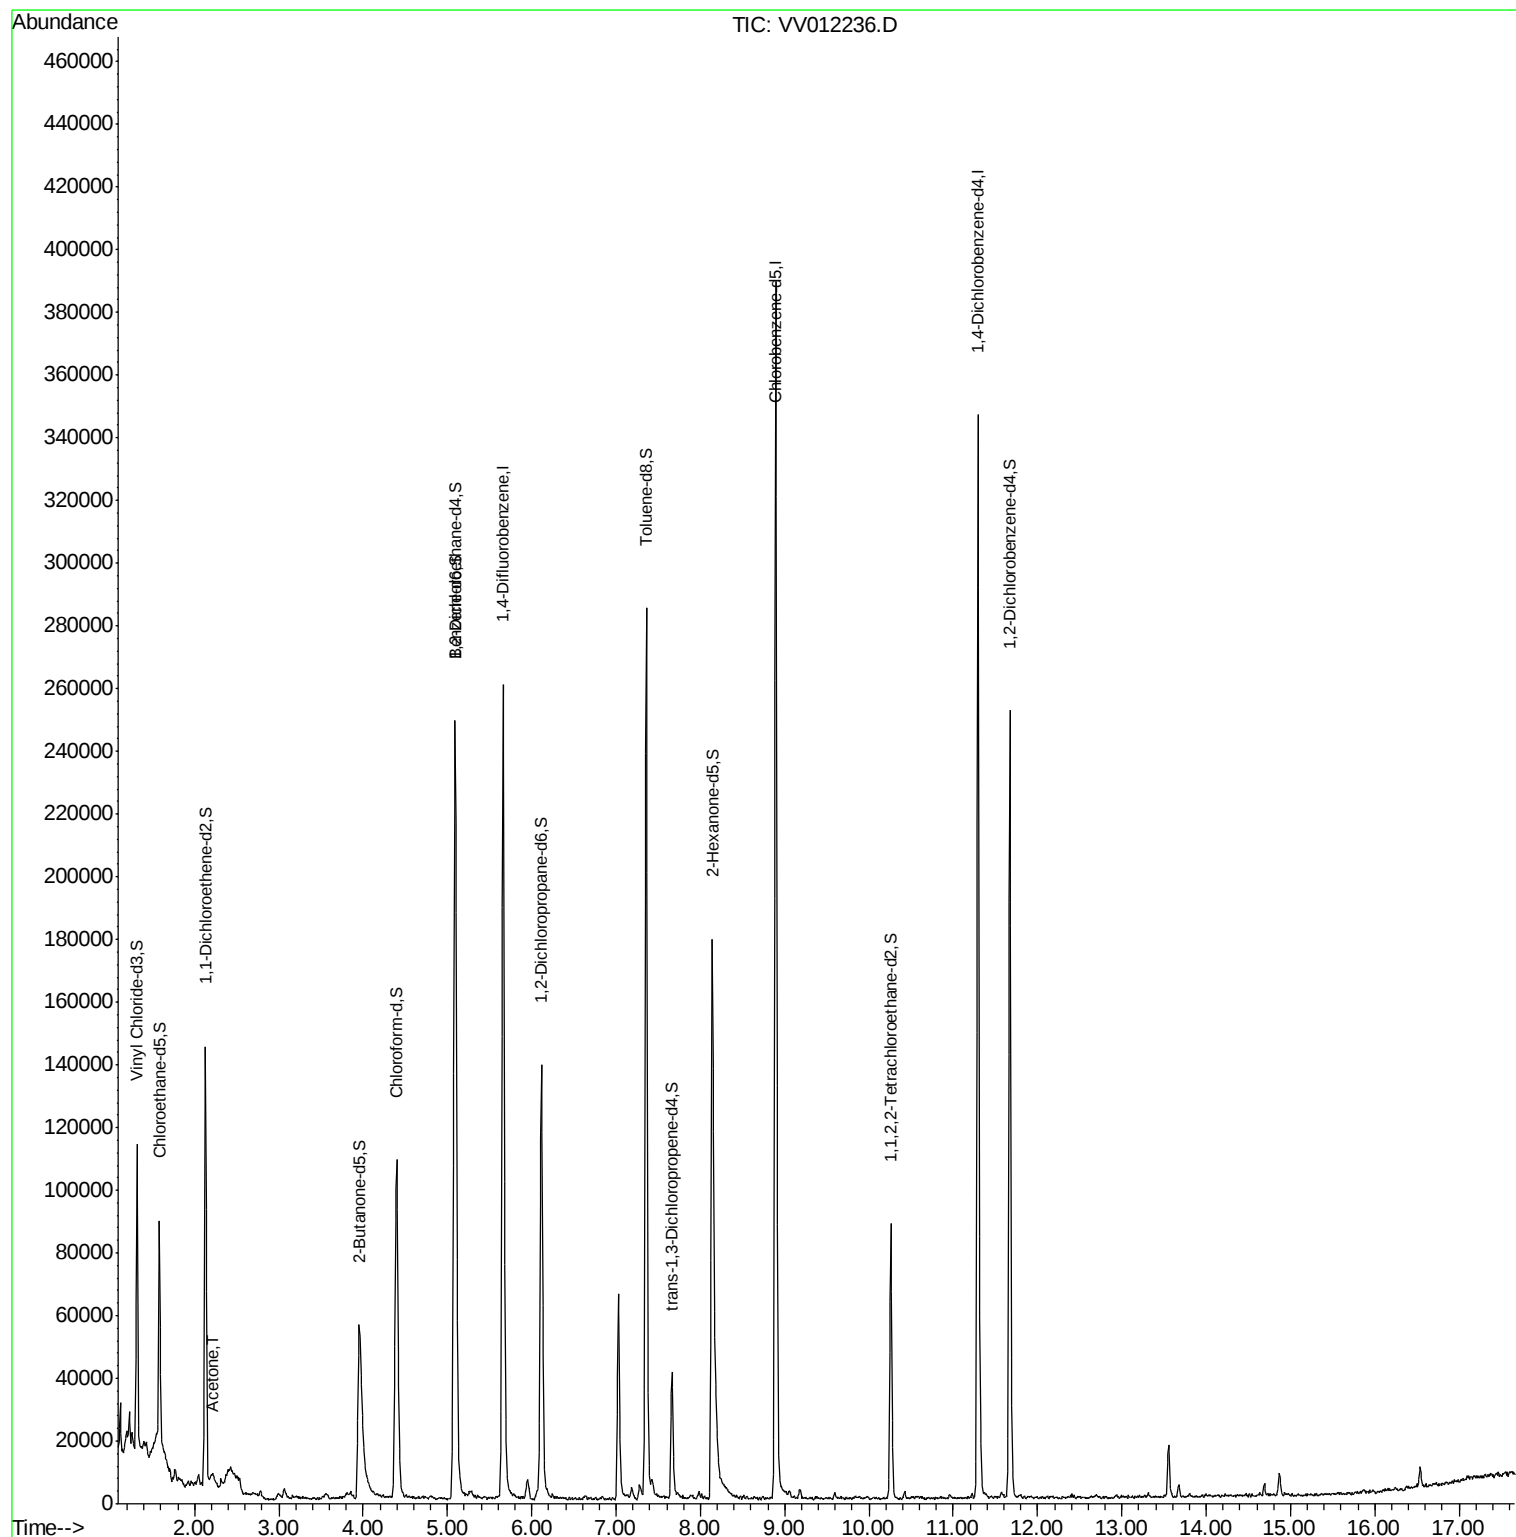

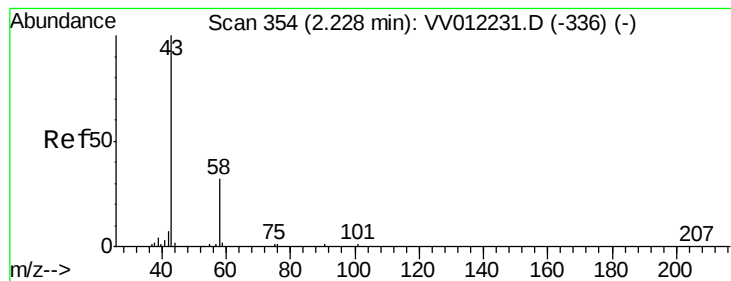

#13
 Acetone
 Concen: 3.523 ug/L
 RT: 2.22 min Scan# 351
 Delta R.T. -0.01 min
 Lab File: VV012236.D
 Acq: 14 Aug 2019 15:52

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA0

Tgt Ion: 43 Resp: 6455
 Ion Ratio Lower Upper
 43 100
 58 33.5 0.0 59.4

