


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV081419\
Data File : VV012230.D
Acq On : 14 Aug 2019 09:15
Operator : SY/MD
Sample : BFB47
Misc : 25mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB47

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Aug 16 10:50:59 2019

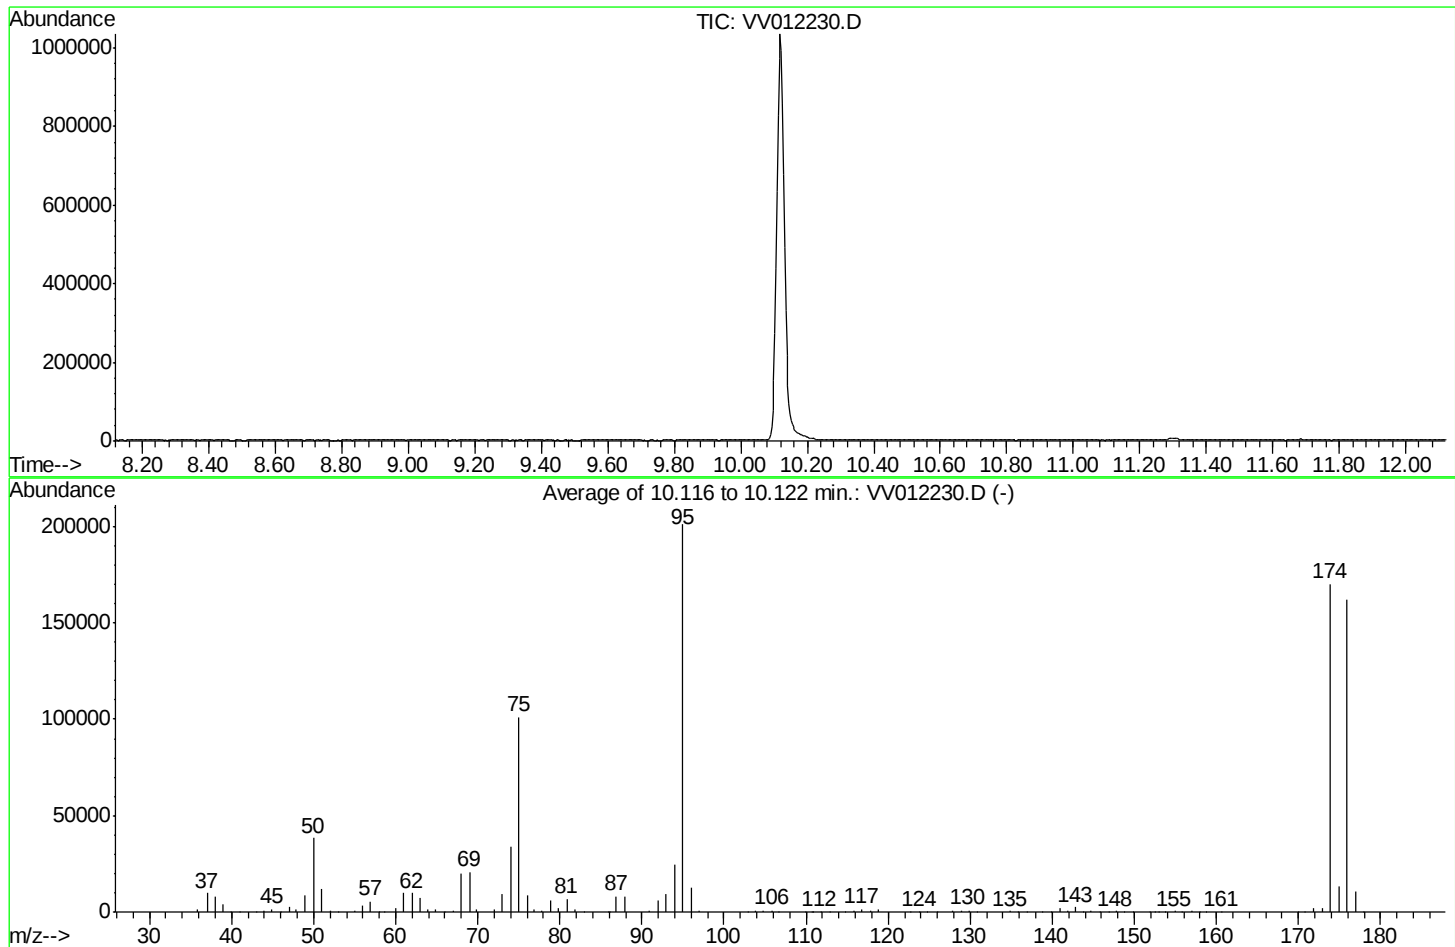

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	38360	PASS
75	95	30	80	50.3	101168	PASS
95	95	100	100	100.0	201130	PASS
96	95	5	9	6.4	12952	PASS
173	174	0.00	2	1.3	2141	PASS
174	95	50	120	84.6	170240	PASS
175	174	5	9	7.6	12986	PASS
176	174	95	101	95.1	161941	PASS
177	176	5	9	6.6	10703	PASS

m/z	Abundance
36.00	1631.0
37.00	9530.0
38.00	8336.0
39.00	4093.0
39.90	817.0
41.00	154.0
42.90	218.0
43.90	1884.0
44.90	1732.0
45.90	285.0
47.00	2246.0
47.90	1203.0
49.00	8202.0
50.00	38008.0
51.00	12530.0
52.00	563.0
53.00	193.0
54.90	472.0
55.90	3101.0
56.90	5610.0
58.00	371.0
60.00	1859.0
61.00	9504.0
62.00	9714.0
63.00	7306.0
63.90	1210.0
64.90	1152.0
66.00	182.0
67.00	677.0
68.00	19832.0
69.00	20264.0
69.90	1436.0
71.90	978.0
72.90	9210.0
74.00	34104.0
75.00	100568.0
76.00	8703.0
76.90	1092.0
77.70	750.0
78.90	6129.0
79.80	1843.0
80.90	6774.0
81.90	1551.0
83.00	242.0
85.90	270.0
86.90	7736.0
87.90	7554.0
90.90	844.0
91.90	5669.0
92.90	9092.0
94.00	23696.0
95.00	195712.0
96.00	12697.0
97.00	417.0
102.90	113.0
103.80	971.0
104.80	432.0
105.90	921.0
106.70	265.0
109.90	101.0
110.70	190.0
111.70	157.0
112.80	194.0
114.70	195.0
115.90	694.0
116.80	1463.0
117.80	818.0
118.90	1210.0
123.80	147.0
125.90	109.0
127.80	622.0
128.90	340.0
129.80	673.0
130.80	292.0
134.90	439.0
136.80	278.0
138.80	114.0
140.90	2041.0
141.90	382.0
142.90	2272.0
143.80	161.0
144.80	488.0
145.80	273.0
146.90	237.0
147.80	418.0
148.80	150.0
149.90	208.0
153.80	177.0
155.00	468.0
155.80	196.0
157.00	352.0
157.90	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

158.80	250.0
160.60	220.0
169.90	143.0
170.80	323.0
171.90	1990.0
172.90	2050.0
173.90	162688.0
174.90	12447.0
175.90	154304.0
176.90	10555.0
177.90	298.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

m/z	Abundance
36.00	1624.0
37.00	10119.0
38.00	8527.0
39.00	4075.0
39.90	893.0
41.00	159.0
42.90	255.0
43.90	1849.0
45.00	1747.0
45.90	301.0
47.00	2434.0
47.90	1240.0
49.00	8731.0
50.00	39936.0
51.00	12668.0
52.00	637.0
53.00	185.0
55.00	488.0
55.90	3416.0
57.00	5531.0
58.00	330.0
60.00	1929.0
60.90	10120.0
62.00	10328.0
63.00	7690.0
63.90	1169.0
64.90	1152.0
66.00	173.0
67.00	715.0
68.00	20864.0
69.00	21312.0
69.90	1547.0
72.00	1095.0
72.90	9762.0
74.00	35128.0
75.00	104576.0
76.00	9058.0
76.90	1217.0
77.70	847.0
78.90	6451.0
79.90	1808.0
80.90	7099.0
81.90	1487.0
83.00	275.0
85.90	280.0
86.90	8225.0
87.90	7880.0
90.80	847.0
91.90	6153.0
92.90	9606.0
94.00	25272.0
95.00	208000.0
96.00	13309.0
96.90	443.0
103.80	925.0
104.80	404.0
105.90	980.0
106.70	232.0
109.80	160.0
110.70	206.0
111.70	179.0
112.80	239.0
114.70	209.0
115.80	761.0
116.80	1524.0
117.90	782.0
118.90	1338.0
122.70	104.0
123.80	152.0
125.90	105.0
127.80	639.0
129.00	394.0
129.80	737.0
130.80	342.0
134.90	507.0
135.80	126.0
136.90	324.0
139.90	126.0
140.90	2241.0
141.80	397.0
142.80	2457.0
143.80	146.0
144.70	478.0
145.80	314.0
146.90	187.0
147.80	508.0
148.80	166.0
149.90	159.0
151.80	127.0
152.50	114.0
152.90	152.0
153.70	163.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

155.00	546.0
155.70	236.0
156.90	385.0
157.90	121.0
158.80	256.0
160.60	219.0
169.90	175.0
170.80	315.0
171.90	1910.0
173.00	2200.0
173.90	176128.0
174.90	13436.0
175.90	167424.0
176.90	11108.0
177.90	305.0
207.00	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

m/z	Abundance
35.90	1538.0
37.00	9510.0
38.00	7830.0
39.00	3695.0
39.90	864.0
41.00	169.0
43.00	240.0
43.90	1711.0
45.00	1723.0
46.00	293.0
47.00	2396.0
47.90	1166.0
49.00	8357.0
50.00	37136.0
51.00	11379.0
52.00	578.0
52.90	222.0
55.00	504.0
55.90	3189.0
57.00	5058.0
58.00	224.0
58.60	154.0
59.90	1819.0
60.90	9347.0
62.00	9553.0
63.00	7322.0
63.90	1094.0
64.90	1155.0
66.00	174.0
67.00	672.0
68.00	19824.0
69.00	20280.0
69.90	1499.0
72.00	1098.0
72.90	9161.0
74.00	32968.0
75.00	98360.0
76.00	8396.0
76.90	1226.0
77.80	783.0
78.90	6219.0
79.90	1734.0
80.90	6628.0
81.80	1407.0
83.00	235.0
86.10	297.0
86.90	8030.0
87.90	7704.0
90.80	792.0
91.90	6011.0
92.90	9155.0
94.00	24256.0
95.00	199680.0
96.00	12850.0
96.90	405.0
103.80	798.0
104.80	327.0
105.90	897.0
106.70	197.0
109.80	198.0
110.90	216.0
111.80	175.0
112.80	264.0
114.80	214.0
115.80	702.0
116.80	1379.0
117.90	724.0
118.80	1260.0
122.70	109.0
123.80	137.0
124.70	109.0
127.80	654.0
128.90	386.0
129.80	712.0
130.80	333.0
134.90	512.0
135.80	132.0
136.90	340.0
139.70	134.0
140.90	2198.0
141.80	351.0
142.80	2363.0
143.80	135.0
144.70	414.0
145.90	309.0
146.90	126.0
147.80	536.0
148.80	156.0
149.90	125.0
151.80	148.0
152.50	102.0
152.90	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

153.70	131.0
154.90	579.0
155.70	231.0
156.90	348.0
157.90	105.0
158.80	222.0
160.70	211.0
169.90	172.0
170.80	268.0
171.90	1902.0
173.00	2174.0
173.90	171904.0
174.90	13075.0
175.90	164096.0
176.90	10448.0
177.90	292.0
207.00	197.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

m/z	Abundance
35.90	111.0
38.70	124.0
39.80	721.0
40.90	142.0
41.80	114.0
44.00	803.0
44.80	103.0
45.70	105.0
77.80	161.0
207.00	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47