
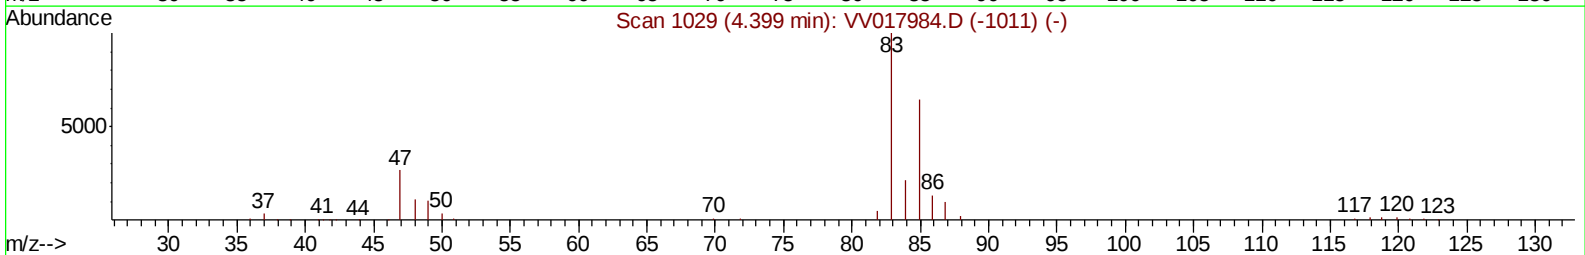
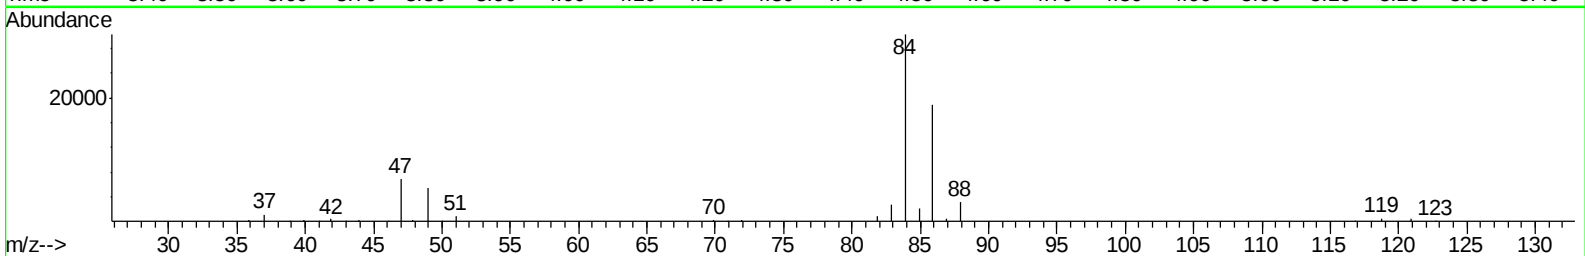


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081420\
Data File : VV017995.D
Acq On : 14 Aug 2020 14:17
Operator : SY/MD
Sample : L3665-12
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Aug 17 01:36:20 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Aug 17 01:31:40 2020
Response via : Initial Calibration

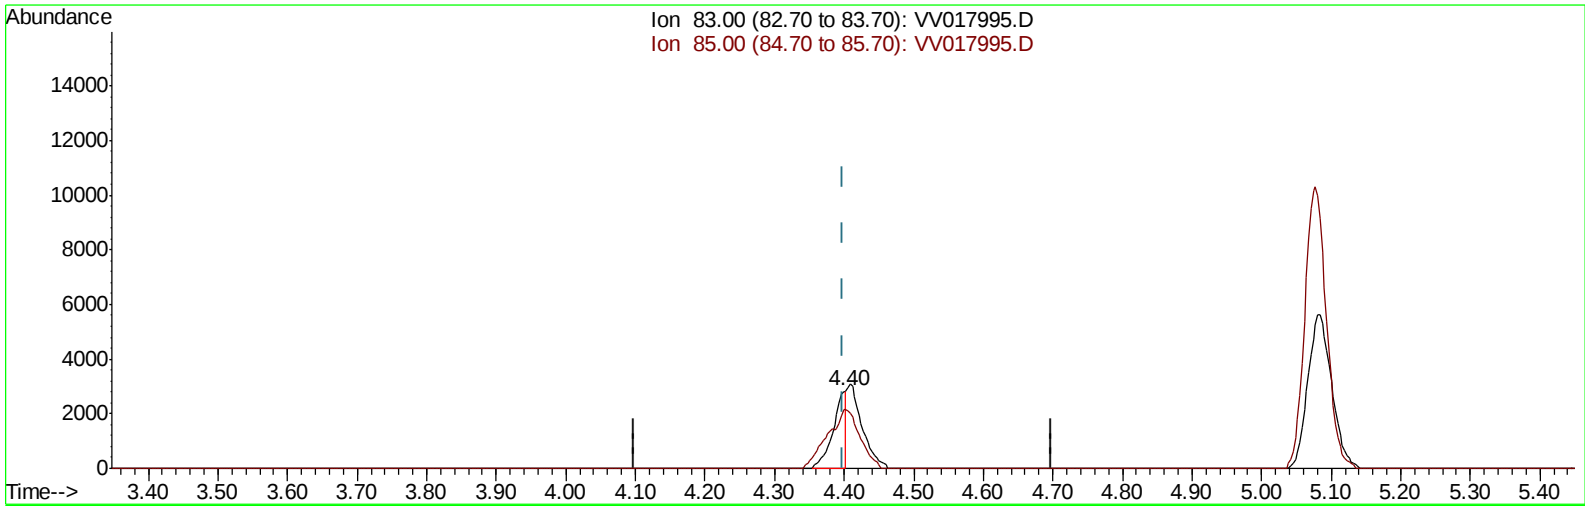

TIC: VV017995.D

(25) Chloroform (T)

4.399min (-0.000) 1.06ug/L

response 3730

Ion	Exp%	Act%
83.00	100	100
85.00	65.00	75.73
0.00	0.00	0.00
0.00	0.00	0.00