
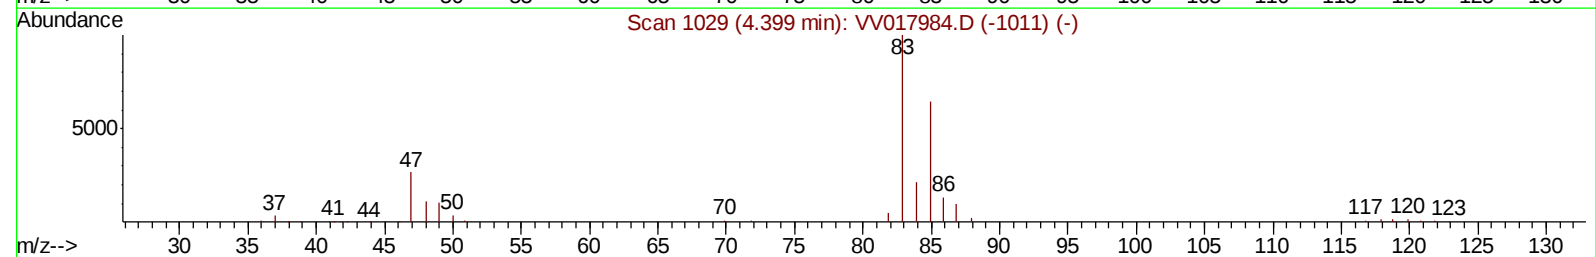
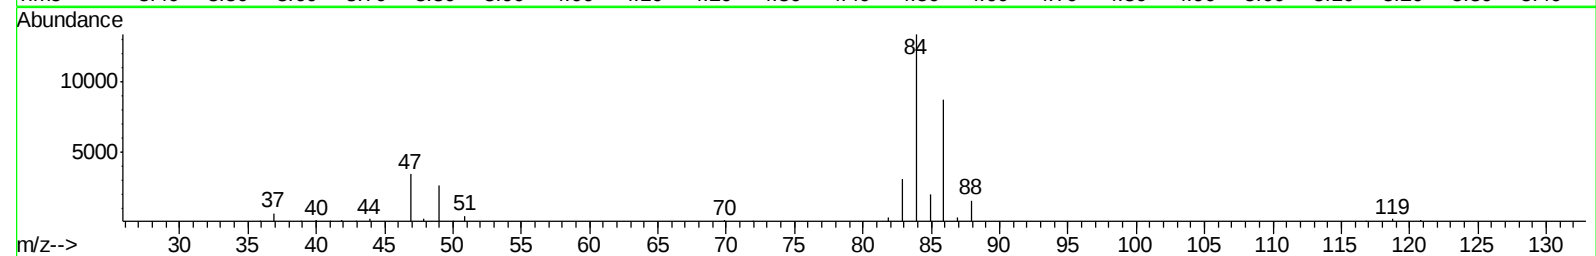


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081420\
 Data File : VV017995.D
 Acq On : 14 Aug 2020 14:17
 Operator : SY/MD
 Sample : L3665-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Aug 17 01:36:20 2020
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Aug 17 01:31:40 2020
 Response via : Initial Calibration

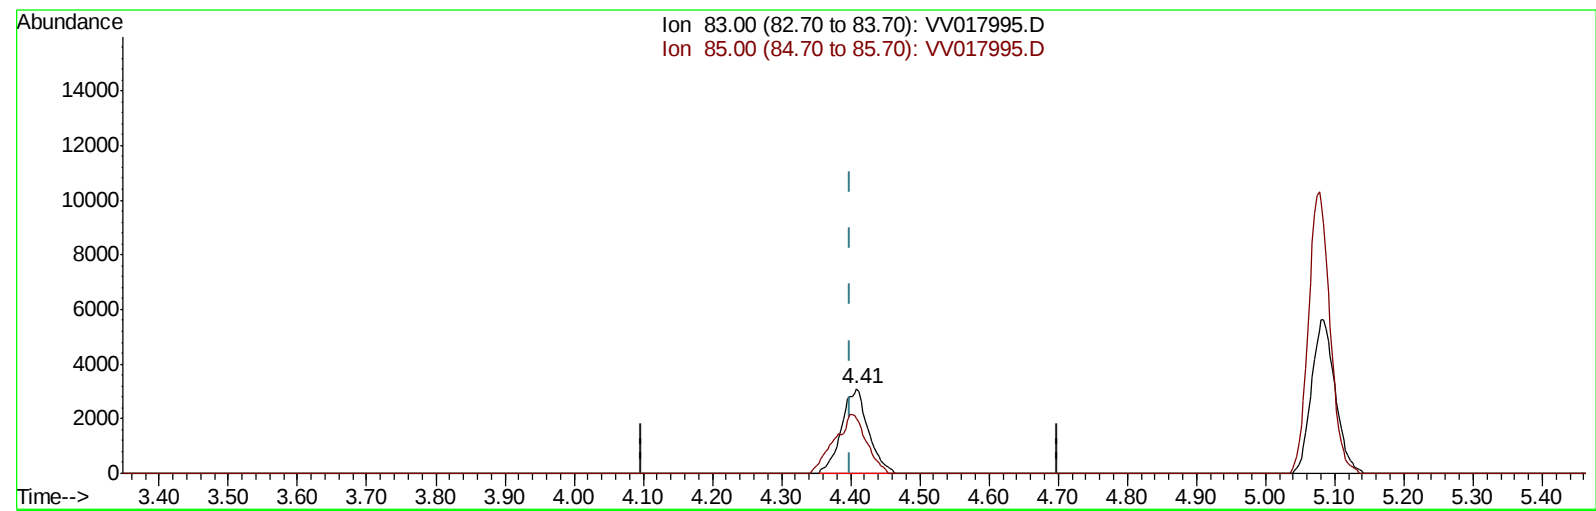

TIC: VV017995.D

(25) Chloroform (T)

4.409min (+0.010) 2.38ug/L m

response 8358

Ion	Exp%	Act%
83.00	100	100
85.00	65.00	64.47
0.00	0.00	0.00
0.00	0.00	0.00