

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081420\
 Data File : VV018005.D
 Acq On : 14 Aug 2020 18:36
 Operator : SY/MD
 Sample : L3665-07DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4L39DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	62	70	85	rVB2	214505	227308	19.81%	2.298%
2	1.576	143	151	167	rBV	137205	155858	13.58%	1.576%
3	2.119	310	320	350	rVB	274707	419761	36.58%	4.244%
4	2.312	374	380	389	rVB3	783	1072	0.09%	0.011%
5	2.399	404	407	410	rBV2	170	144	0.01%	0.001%
6	2.460	421	426	432	rVB2	316	388	0.03%	0.004%
7	2.528	432	447	448	rBV3	3022	4283	0.37%	0.043%
8	2.778	514	525	541	rBV	23168	41829	3.65%	0.423%
9	3.309	686	690	696	rBV2	141	151	0.01%	0.002%
10	3.434	726	729	735	rVB2	194	191	0.02%	0.002%
11	3.505	748	751	753	rBV2	171	109	0.01%	0.001%
12	3.756	824	829	832	rBV2	226	205	0.02%	0.002%
13	3.794	832	841	849	rVB4	1285	2105	0.18%	0.021%
14	3.936	865	885	920	rBV2	413595	1147570	100.00%	11.603%
15	4.219	971	973	978	rVB2	407	239	0.02%	0.002%
16	4.306	997	1000	1002	rBV2	192	135	0.01%	0.001%
17	4.373	1005	1021	1055	rVV	172825	428048	37.30%	4.328%
18	4.531	1067	1070	1074	rBV2	282	193	0.02%	0.002%
19	4.560	1077	1079	1084	rVB2	255	197	0.02%	0.002%
20	4.698	1115	1122	1124	rBV3	917	835	0.07%	0.008%
21	4.788	1146	1150	1158	rVB3	464	659	0.06%	0.007%
22	4.962	1198	1204	1206	rBV3	319	274	0.02%	0.003%
23	5.071	1220	1238	1271	rBV2	431319	1103513	96.16%	11.158%
24	5.238	1288	1290	1295	rVB	243	157	0.01%	0.002%
25	5.270	1296	1300	1301	rBV2	392	237	0.02%	0.002%
26	5.347	1317	1324	1325	rBV5	877	866	0.08%	0.009%
27	5.441	1351	1353	1356	rVB2	182	125	0.01%	0.001%
28	5.524	1375	1379	1381	rBV3	189	173	0.02%	0.002%
29	5.640	1403	1415	1441	rBV	317586	621530	54.16%	6.284%
30	5.875	1485	1488	1493	rBV2	267	186	0.02%	0.002%
31	5.936	1493	1507	1534	rBV2	260600	520103	45.32%	5.259%
32	6.093	1543	1556	1585	rBV	247460	504377	43.95%	5.100%
33	6.235	1594	1600	1604	rBV4	404	534	0.05%	0.005%
34	6.312	1619	1624	1628	rBV3	225	231	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081420\
 Data File : VV018005.D
 Acq On : 14 Aug 2020 18:36
 Operator : SY/MD
 Sample : L3665-07DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4L39DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis

35	6.502	1682	1683	1690	rVB2	222	130	0.01%	0.001%
36	6.682	1735	1739	1745	rVB3	246	220	0.02%	0.002%
37	6.714	1745	1749	1753	rBV2	124	140	0.01%	0.001%
38	6.916	1804	1812	1816	rBV	216	285	0.02%	0.003%
39	7.006	1828	1840	1864	rBV	127402	227858	19.86%	2.304%
40	7.193	1896	1898	1903	rVB2	243	124	0.01%	0.001%
41	7.293	1924	1929	1930	rBV	205	149	0.01%	0.002%
42	7.338	1930	1943	1968	rBV	499793	860344	74.97%	8.699%
43	7.559	2009	2012	2017	rVB3	227	153	0.01%	0.002%
44	7.643	2026	2038	2063	rBV	91942	157509	13.73%	1.593%
45	7.997	2136	2148	2169	rBV	147954	248755	21.68%	2.515%
46	8.109	2172	2183	2222	rBV	202830	393380	34.28%	3.978%
47	8.293	2239	2240	2243	rBV	285	177	0.02%	0.002%
48	8.354	2257	2259	2263	rVB2	343	217	0.02%	0.002%
49	8.399	2271	2273	2278	rVV3	272	249	0.02%	0.003%
50	8.431	2280	2283	2284	rVV	508	259	0.02%	0.003%
51	8.447	2284	2288	2299	rVB4	738	1018	0.09%	0.010%
52	8.508	2299	2307	2310	rBV2	82	126	0.01%	0.001%
53	8.871	2408	2420	2446	rBV	483449	780752	68.04%	7.894%
54	9.042	2470	2473	2477	rVB2	295	286	0.02%	0.003%
55	9.080	2483	2485	2490	rVB2	168	133	0.01%	0.001%
56	9.241	2529	2535	2542	rVB2	149	218	0.02%	0.002%
57	9.283	2542	2548	2550	rBV2	142	158	0.01%	0.002%
58	9.334	2558	2564	2567	rBV2	98	121	0.01%	0.001%
59	9.498	2610	2615	2618	rBV	130	138	0.01%	0.001%
60	9.672	2665	2669	2675	rBV	124	107	0.01%	0.001%
61	9.775	2695	2701	2704	rVB2	150	156	0.01%	0.002%
62	9.829	2713	2718	2722	rBV2	94	128	0.01%	0.001%
63	10.093	2796	2800	2804	rBV2	120	133	0.01%	0.001%
64	10.238	2833	2845	2865	rBV	299126	468343	40.81%	4.735%
65	10.395	2890	2894	2898	rBV3	291	308	0.03%	0.003%
66	10.540	2936	2939	2946	rVB2	175	187	0.02%	0.002%
67	10.682	2980	2983	2989	rVV2	171	176	0.02%	0.002%
68	10.762	3002	3008	3014	rVB2	254	228	0.02%	0.002%
69	10.997	3077	3081	3085	rBV	185	153	0.01%	0.002%
70	11.035	3085	3093	3098	rVV2	177	240	0.02%	0.002%
71	11.212	3146	3148	3153	rBV2	208	131	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081420\
 Data File : VV018005.D
 Acq On : 14 Aug 2020 18:36
 Operator : SY/MD
 Sample : L3665-07DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4L39DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis

72	11.270	3154	3166	3190	rBV	484219	745805	64.99%	7.541%
73	11.376	3196	3199	3204	rVB4	363	344	0.03%	0.003%
74	11.579	3259	3262	3269	rVB3	220	183	0.02%	0.002%
75	11.646	3269	3283	3305	rBV	524110	812725	70.82%	8.218%
76	11.813	3332	3335	3338	rVB2	193	161	0.01%	0.002%
77	11.833	3338	3341	3343	rBV	268	172	0.01%	0.002%
78	11.845	3343	3345	3348	rBV	159	121	0.01%	0.001%
79	11.942	3371	3375	3378	rBV	207	211	0.02%	0.002%
80	11.977	3381	3386	3390	rVB3	272	245	0.02%	0.002%
81	11.997	3390	3392	3399	rBV	224	201	0.02%	0.002%
82	12.222	3459	3462	3465	rVV	186	125	0.01%	0.001%
83	12.251	3469	3471	3474	rVV	237	183	0.02%	0.002%
84	12.270	3475	3477	3484	rVB2	347	390	0.03%	0.004%
85	12.752	3624	3627	3630	rBV2	142	114	0.01%	0.001%
86	13.427	3834	3837	3841	rVB2	223	165	0.01%	0.002%
87	13.466	3845	3849	3852	rBV2	183	153	0.01%	0.002%
88	13.987	4009	4011	4015	rVB	237	119	0.01%	0.001%
89	14.048	4027	4030	4031	rBV	201	110	0.01%	0.001%
90	14.093	4039	4044	4046	rBV2	275	240	0.02%	0.002%
91	14.167	4064	4067	4071	rVB2	241	151	0.01%	0.002%
92	14.189	4072	4074	4077	rBV2	242	112	0.01%	0.001%
93	14.279	4100	4102	4108	rBB2	243	221	0.02%	0.002%
94	14.328	4114	4117	4119	rBV	199	126	0.01%	0.001%
95	14.424	4143	4147	4149	rBV3	256	216	0.02%	0.002%
96	14.492	4166	4168	4170	rBV	243	148	0.01%	0.001%
97	14.620	4205	4208	4210	rBV2	176	119	0.01%	0.001%
98	14.771	4253	4255	4258	rVB2	370	180	0.02%	0.002%
99	14.787	4258	4260	4263	rBV3	193	138	0.01%	0.001%
100	15.112	4359	4361	4364	rBV2	208	158	0.01%	0.002%


Sum of corrected areas: 9890111

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081420\
Data File : VV018005.D
Acq On : 14 Aug 2020 18:36
Operator : SY/MD
Sample : L3665-07DL 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F4L39DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

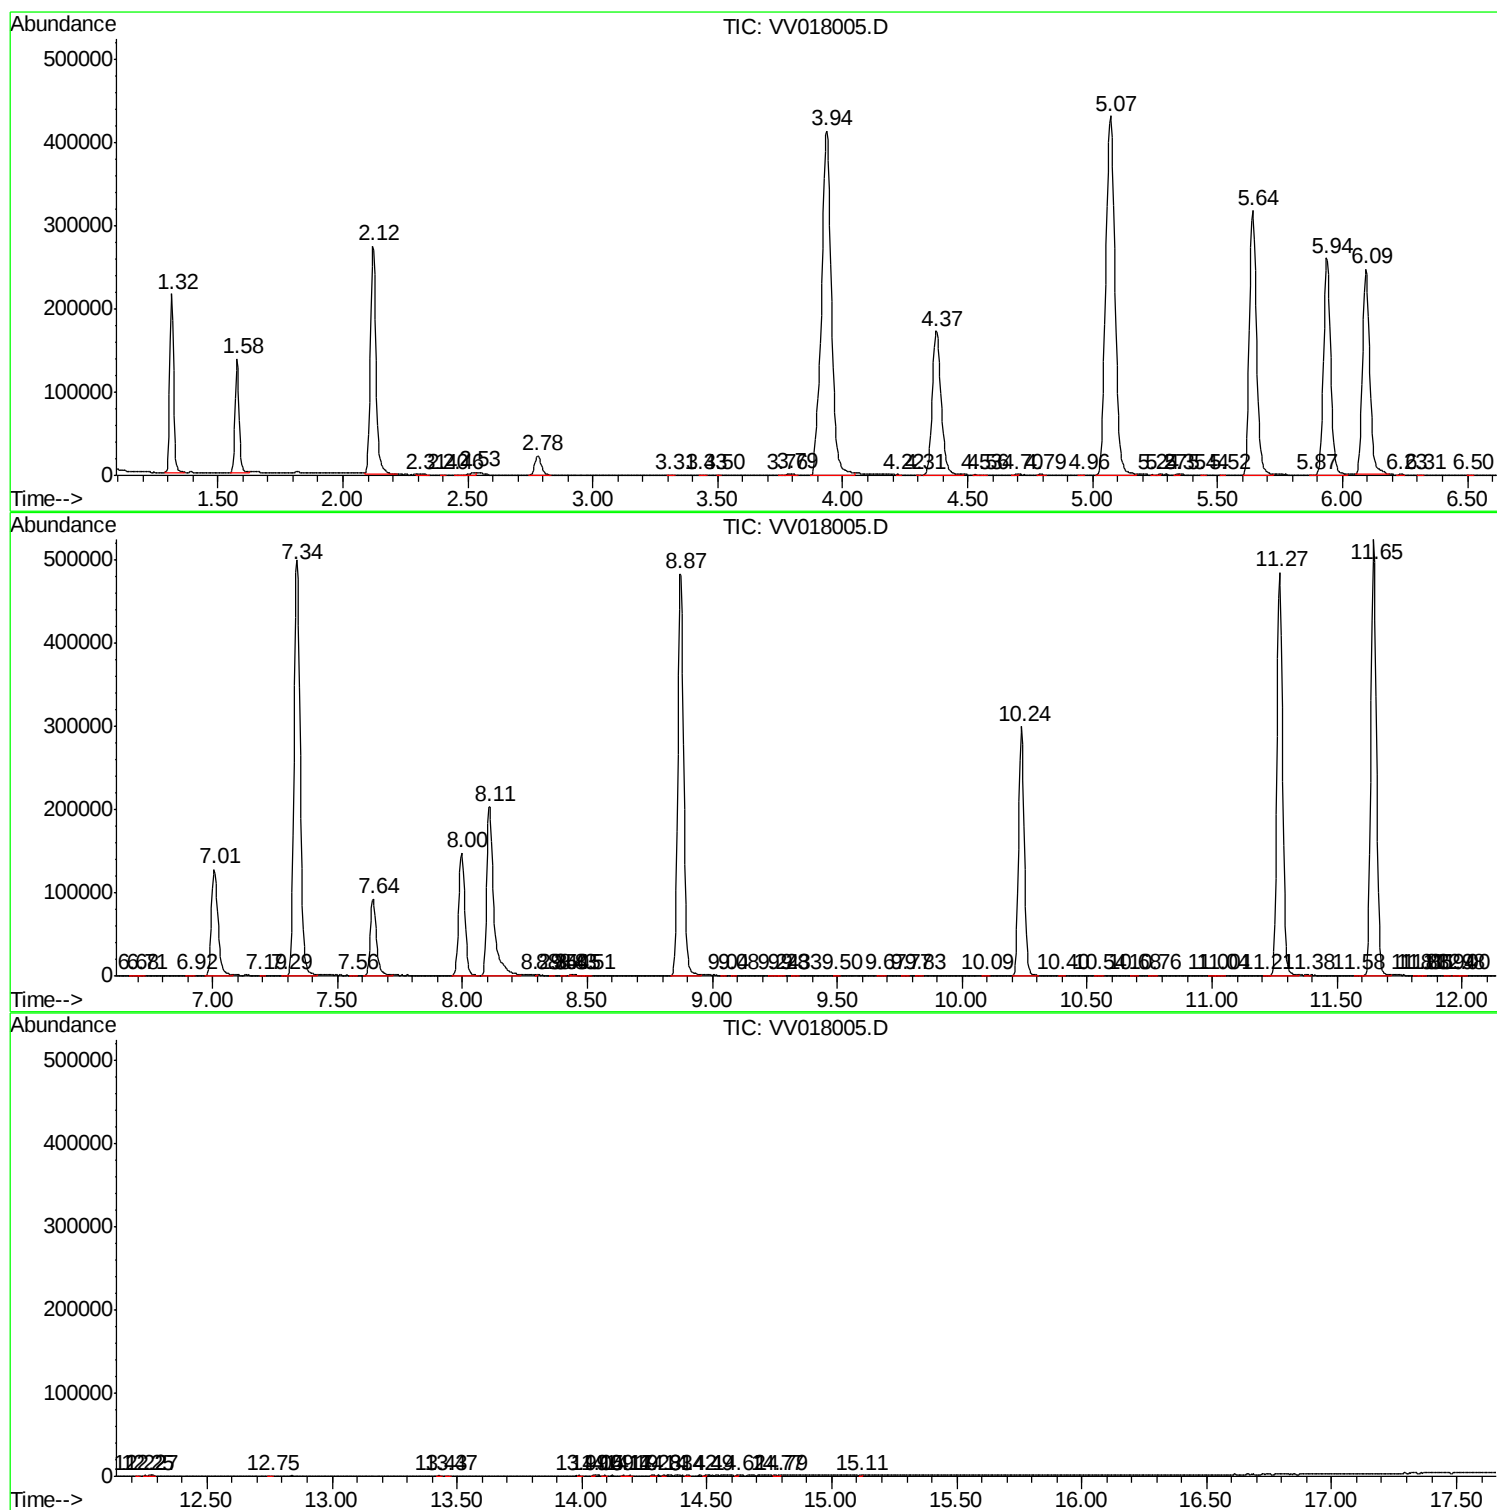

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081420\
Data File : VV018005.D
Acq On : 14 Aug 2020 18:36
Operator : SY/MD
Sample : L3665-07DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4L39DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081420\
Data File : VV018005.D
Acq On : 14 Aug 2020 18:36
Operator : SY/MD
Sample : L3665-07DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4L39DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc