

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081420\
 Data File : VV018006.D
 Acq On : 14 Aug 2020 18:59
 Operator : SY/MD
 Sample : L3665-10DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4L71DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	83	rVB2	164537	173301	20.68%	2.404%
2	1.576	144	151	167	rBV	93624	111545	13.31%	1.548%
3	2.122	311	321	343	rVB	180860	283716	33.86%	3.936%
4	2.524	439	446	456	rVB3	2516	3766	0.45%	0.052%
5	2.630	476	479	481	rBV3	215	138	0.02%	0.002%
6	2.782	517	526	540	rVB3	6830	12155	1.45%	0.169%
7	3.055	606	611	618	rBV2	200	236	0.03%	0.003%
8	3.421	722	725	728	rBV	86	52	0.01%	0.001%
9	3.441	728	731	732	rBV	85	52	0.01%	0.001%
10	3.601	775	781	785	rBV2	139	168	0.02%	0.002%
11	3.714	813	816	822	rVB2	113	114	0.01%	0.002%
12	3.807	842	845	847	rBV	110	72	0.01%	0.001%
13	3.936	865	885	923	rBV2	176876	578442	69.02%	8.025%
14	4.376	1005	1022	1047	rBV	138908	345848	41.27%	4.798%
15	4.550	1074	1076	1077	rBV	212	93	0.01%	0.001%
16	4.585	1085	1087	1089	rBV2	56	31	0.00%	0.000%
17	4.656	1106	1109	1115	rVB	169	152	0.02%	0.002%
18	4.704	1116	1124	1126	rBV	89	139	0.02%	0.002%
19	4.727	1128	1131	1134	rBV2	142	117	0.01%	0.002%
20	4.775	1143	1146	1151	rBV	95	90	0.01%	0.001%
21	4.801	1151	1154	1156	rBV2	84	53	0.01%	0.001%
22	4.891	1179	1182	1184	rBV	88	54	0.01%	0.001%
23	5.071	1220	1238	1268	rBV2	324421	838023	100.00%	11.627%
24	5.344	1322	1323	1324	rVB2	118	23	0.00%	0.000%
25	5.357	1324	1327	1329	rBV2	124	91	0.01%	0.001%
26	5.370	1329	1331	1332	rVV2	126	53	0.01%	0.001%
27	5.460	1356	1359	1364	rVB2	111	102	0.01%	0.001%
28	5.486	1364	1367	1370	rBV2	100	60	0.01%	0.001%
29	5.502	1370	1372	1375	rVB2	84	43	0.01%	0.001%
30	5.518	1375	1377	1379	rBV2	82	49	0.01%	0.001%
31	5.569	1390	1393	1396	rBV	100	80	0.01%	0.001%
32	5.640	1403	1415	1439	rBV	297560	587490	70.10%	8.151%
33	5.933	1495	1506	1525	rVB4	20883	48411	5.78%	0.672%
34	6.000	1525	1527	1530	rVB2	49	23	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081420\
 Data File : VV018006.D
 Acq On : 14 Aug 2020 18:59
 Operator : SY/MD
 Sample : L3665-10DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4L71DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis

35	6.016	1530	1532	1536	rBV	66	54	0.01%	0.001%
36	6.032	1536	1537	1539	rVB	118	45	0.01%	0.001%
37	6.093	1542	1556	1583	rBV	196890	396067	47.26%	5.495%
38	6.244	1602	1603	1608	rVB2	409	241	0.03%	0.003%
39	6.267	1608	1610	1611	rBV	98	37	0.00%	0.001%
40	6.286	1614	1616	1620	rVB	226	86	0.01%	0.001%
41	6.322	1623	1627	1629	rBV2	149	119	0.01%	0.002%
42	6.379	1642	1645	1649	rBV	66	43	0.01%	0.001%
43	6.476	1668	1675	1679	rBV2	152	187	0.02%	0.003%
44	6.498	1679	1682	1684	rBV	74	43	0.01%	0.001%
45	6.588	1707	1710	1713	rBV	84	65	0.01%	0.001%
46	6.669	1732	1735	1740	rBV	171	163	0.02%	0.002%
47	6.714	1744	1749	1753	rBV	131	135	0.02%	0.002%
48	6.871	1794	1798	1800	rBV2	143	114	0.01%	0.002%
49	7.010	1829	1841	1871	rBV	98077	179699	21.44%	2.493%
50	7.209	1900	1903	1906	rBV	215	154	0.02%	0.002%
51	7.241	1912	1913	1914	rBV	110	25	0.00%	0.000%
52	7.273	1920	1923	1924	rBV2	271	136	0.02%	0.002%
53	7.338	1931	1943	1971	rBV	369938	629642	75.13%	8.736%
54	7.553	2008	2010	2011	rBV	231	95	0.01%	0.001%
55	7.579	2017	2018	2021	rBV	126	45	0.01%	0.001%
56	7.592	2021	2022	2025	rBV	133	74	0.01%	0.001%
57	7.643	2027	2038	2063	rVV	71285	121765	14.53%	1.689%
58	7.781	2078	2081	2087	rVB2	286	257	0.03%	0.004%
59	7.862	2105	2106	2107	rVB2	122	23	0.00%	0.000%
60	7.900	2116	2118	2123	rVB2	195	104	0.01%	0.001%
61	7.926	2123	2126	2130	rBV2	127	100	0.01%	0.001%
62	8.000	2143	2149	2157	rVB3	2311	2999	0.36%	0.042%
63	8.039	2157	2161	2164	rBV2	140	130	0.02%	0.002%
64	8.109	2172	2183	2219	rBV2	179270	355338	42.40%	4.930%
65	8.415	2275	2278	2279	rBV	189	108	0.01%	0.001%
66	8.437	2280	2285	2294	rVB3	981	1416	0.17%	0.020%
67	8.502	2303	2305	2307	rVB	130	52	0.01%	0.001%
68	8.553	2317	2321	2323	rVB	210	128	0.02%	0.002%
69	8.585	2323	2331	2334	rBV2	199	265	0.03%	0.004%
70	8.633	2345	2346	2349	rVB	155	51	0.01%	0.001%
71	8.691	2362	2364	2367	rVV2	146	85	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081420\
 Data File : VV018006.D
 Acq On : 14 Aug 2020 18:59
 Operator : SY/MD
 Sample : L3665-10DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4L71DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis

72	8.707	2367	2369	2371	rVB	165	66	0.01%	0.001%
73	8.756	2379	2384	2385	rBV2	140	114	0.01%	0.002%
74	8.875	2406	2421	2446	rBV	455749	739219	88.21%	10.256%
75	9.206	2520	2524	2528	rBV2	159	138	0.02%	0.002%
76	9.280	2545	2547	2550	rBV	148	105	0.01%	0.001%
77	9.350	2566	2569	2573	rBV2	193	161	0.02%	0.002%
78	9.412	2585	2588	2596	rVB2	150	180	0.02%	0.002%
79	9.469	2603	2606	2609	rBV	140	98	0.01%	0.001%
80	9.649	2660	2662	2665	rBV2	108	58	0.01%	0.001%
81	9.801	2706	2709	2711	rBV	122	70	0.01%	0.001%
82	10.238	2832	2845	2868	rBV	268056	420263	50.15%	5.831%
83	10.344	2876	2878	2884	rVB3	246	193	0.02%	0.003%
84	10.402	2892	2896	2898	rBV2	434	365	0.04%	0.005%
85	11.270	3155	3166	3188	rBV	455195	695356	82.98%	9.648%
86	11.646	3271	3283	3303	rBV	432615	676130	80.68%	9.381%
87	14.193	4072	4075	4077	rBV2	319	235	0.03%	0.003%


Sum of corrected areas: 7207623

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081420\
Data File : VV018006.D
Acq On : 14 Aug 2020 18:59
Operator : SY/MD
Sample : L3665-10DL 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4L71DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

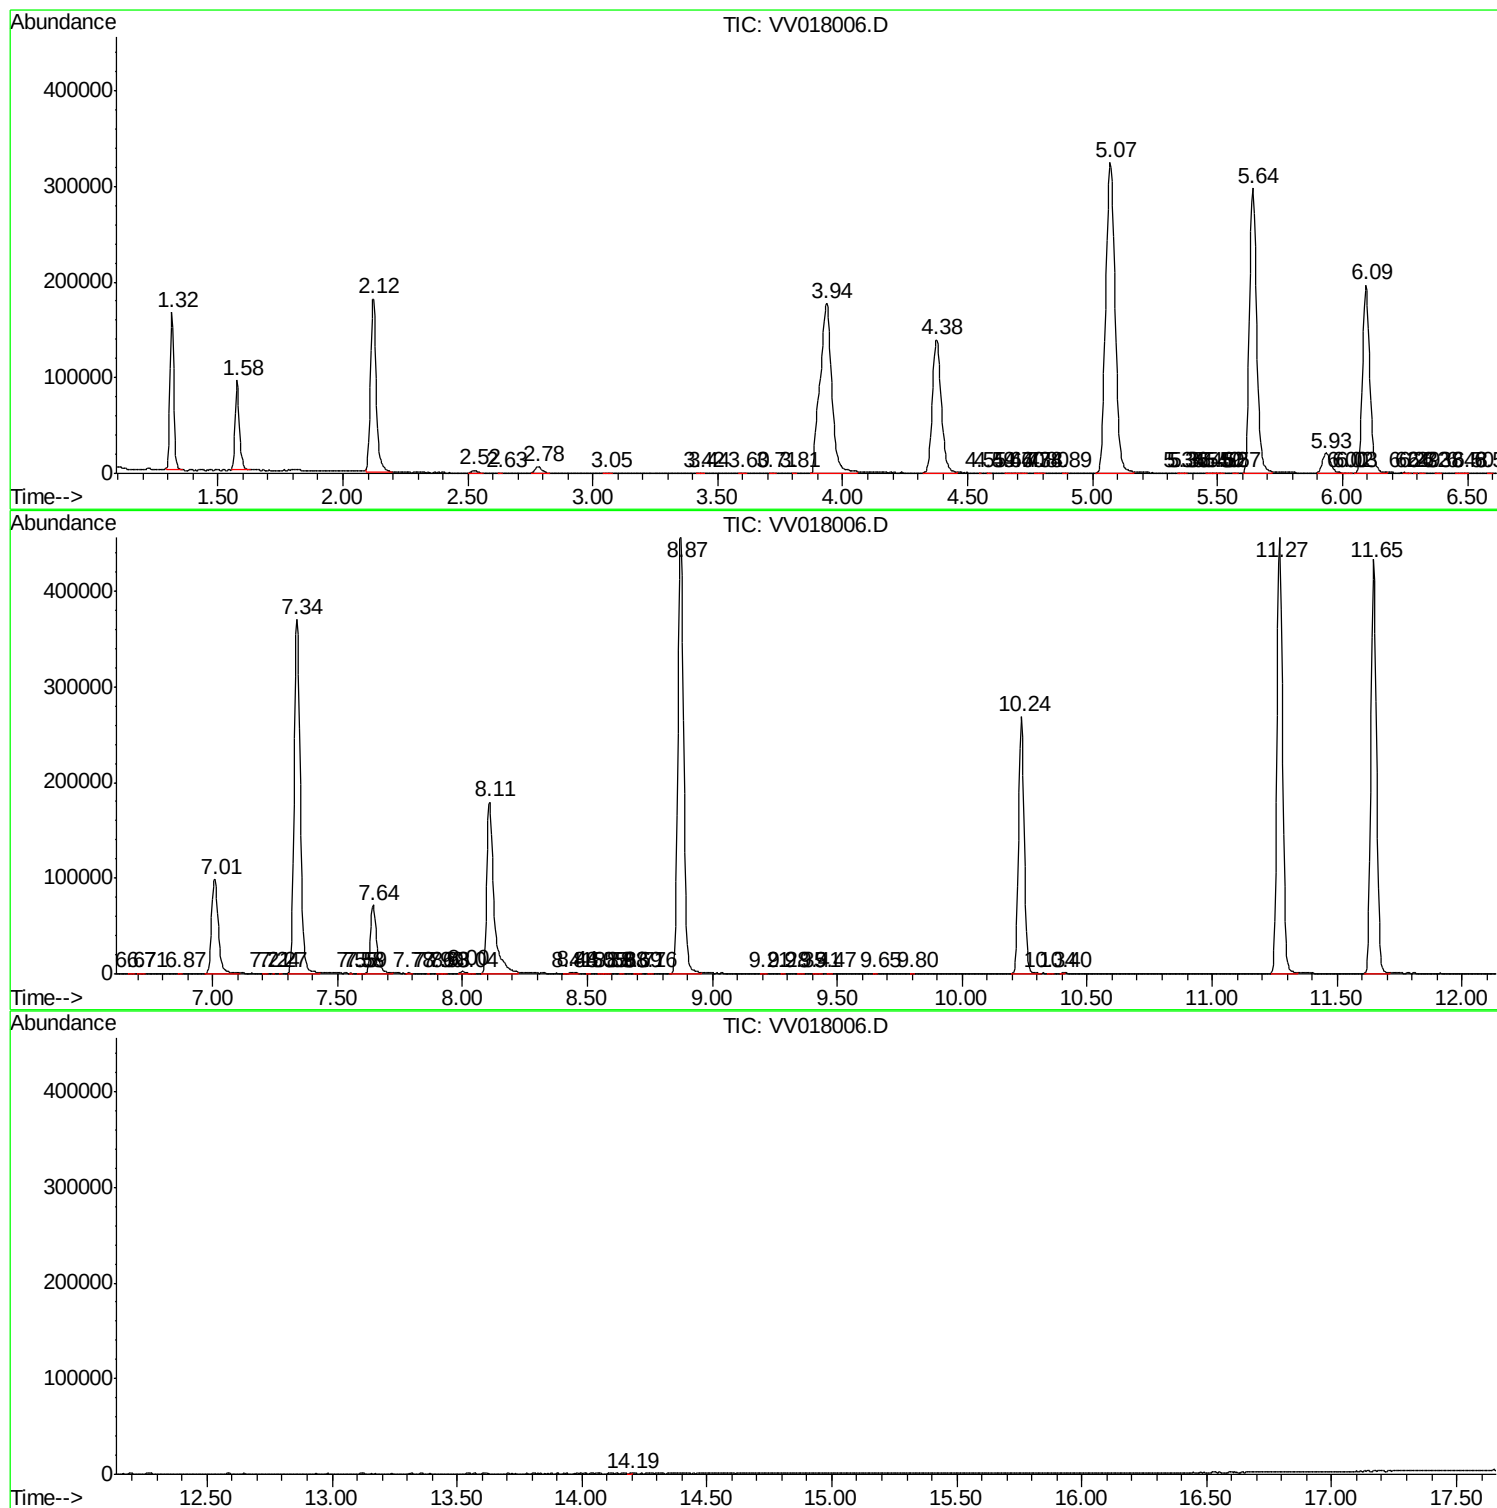

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081420\
Data File : VV018006.D
Acq On : 14 Aug 2020 18:59
Operator : SY/MD
Sample : L3665-10DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4L71DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081420\
Data File : VV018006.D
Acq On : 14 Aug 2020 18:59
Operator : SY/MD
Sample : L3665-10DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4L71DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc