


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV081420\
 Data File : VV017983.D
 Acq On : 14 Aug 2020 09:13
 Operator : SY/MD
 Sample : BFB74
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB74

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 17 01:31:40 2020

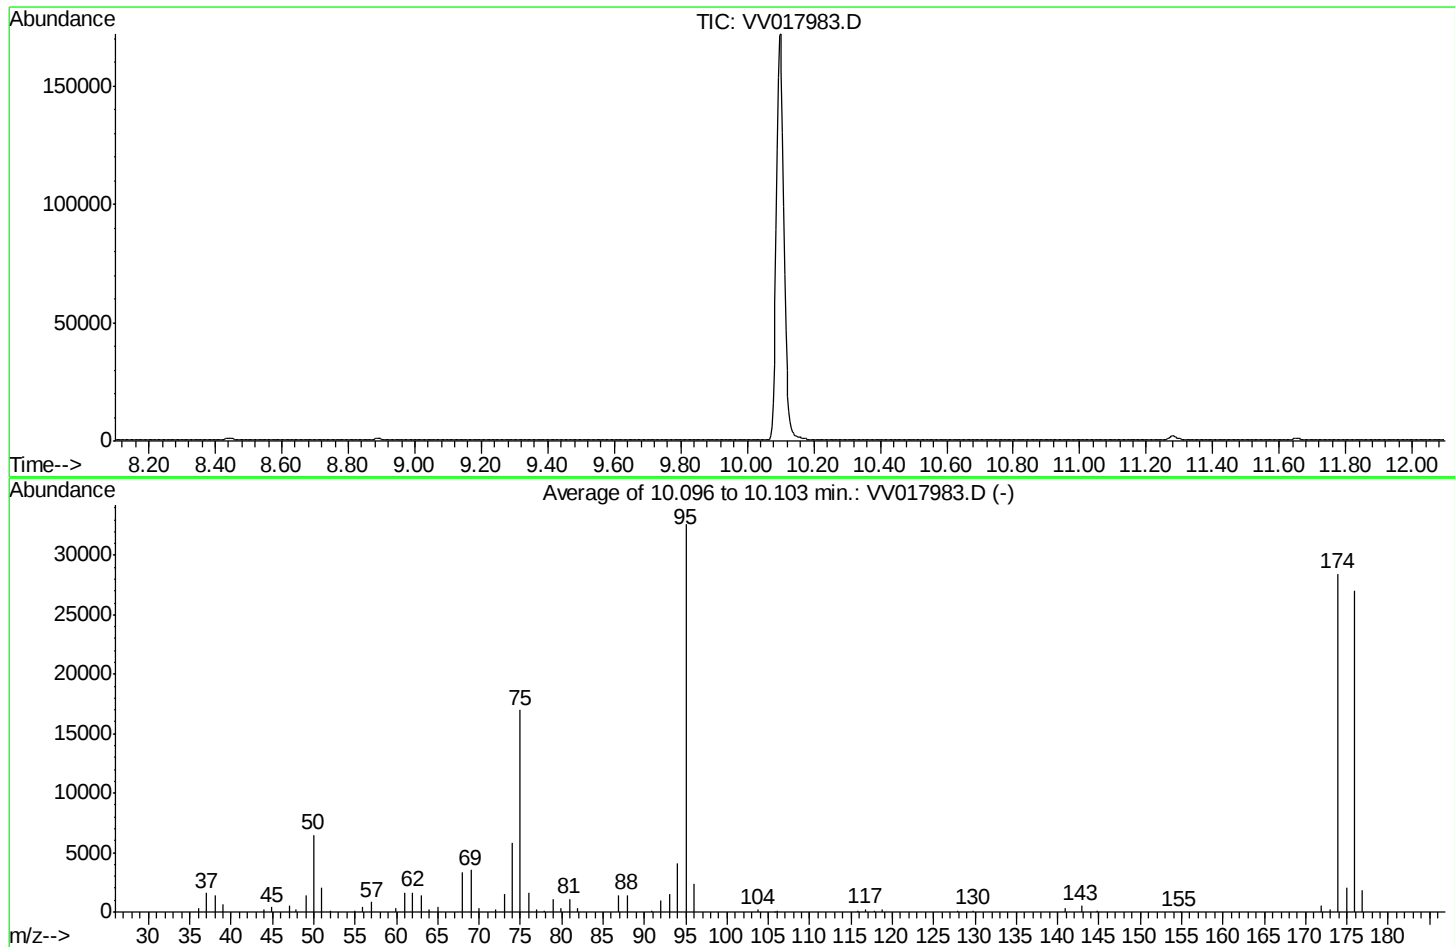

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	6511	PASS
75	95	30	80	52.1	16996	PASS
95	95	100	100	100.0	32618	PASS
96	95	5	9	7.2	2345	PASS
173	174	0.00	2	0.9	254	PASS
174	95	50	120	87.3	28482	PASS
175	174	5	9	7.0	2005	PASS
176	174	95	101	95.0	27058	PASS
177	176	5	9	6.8	1841	PASS

m/z	Abundance
36.00	288.0
37.00	1712.0
38.00	1448.0
39.00	596.0
40.00	177.0
43.90	561.0
44.90	421.0
47.00	575.0
47.90	272.0
49.00	1466.0
50.00	6882.0
51.00	2087.0
52.00	110.0
54.90	129.0
55.90	481.0
57.00	969.0
59.90	326.0
61.00	1718.0
62.00	1644.0
63.00	1486.0
64.00	275.0
65.00	455.0
68.00	3490.0
69.00	3621.0
70.00	343.0
72.00	250.0
73.00	1572.0
74.00	6032.0
75.00	17488.0
76.00	1648.0
76.90	262.0
77.90	122.0
78.90	1109.0
79.90	353.0
80.90	1229.0
81.80	343.0
86.90	1447.0
87.90	1534.0
90.90	123.0
92.00	1032.0
93.00	1539.0
94.00	4308.0
95.00	33528.0
96.00	2535.0
103.80	161.0
105.70	126.0
106.00	128.0
116.00	156.0
116.80	263.0
117.90	154.0
118.80	245.0
127.80	136.0
129.80	188.0
140.80	343.0
142.90	547.0
144.90	179.0
154.80	116.0
171.90	556.0
172.90	367.0
173.90	28368.0
175.00	2137.0
175.90	27488.0
176.90	1831.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
36.00	293.0
37.00	1616.0
38.00	1387.0
39.00	652.0
39.90	174.0
43.90	552.0
44.90	420.0
47.00	564.0
47.90	262.0
49.00	1395.0
50.00	6743.0
51.00	2105.0
52.00	105.0
54.90	134.0
55.90	443.0
57.00	845.0
59.90	313.0
61.00	1669.0
62.00	1681.0
63.00	1409.0
64.00	264.0
65.00	455.0
68.00	3379.0
69.00	3612.0
69.90	334.0
72.00	258.0
73.00	1601.0
74.00	5996.0
75.00	17616.0
76.00	1639.0
76.90	268.0
77.80	110.0
78.90	1153.0
79.90	379.0
80.90	1135.0
81.80	327.0
86.90	1443.0
87.90	1492.0
90.90	130.0
92.00	1027.0
93.00	1512.0
94.00	4211.0
95.00	33616.0
96.00	2421.0
103.80	196.0
106.10	152.0
115.80	157.0
116.80	293.0
117.90	160.0
118.80	258.0
127.90	146.0
129.80	168.0
140.90	340.0
142.90	565.0
144.90	151.0
171.90	573.0
173.00	397.0
173.90	29416.0
175.00	2034.0
175.90	27992.0
176.90	1904.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
36.00	281.0
37.00	1411.0
38.00	1282.0
39.00	642.0
39.90	178.0
43.90	492.0
44.90	365.0
47.00	455.0
47.90	202.0
49.00	1196.0
50.00	5910.0
51.00	1875.0
54.90	125.0
55.90	419.0
57.00	726.0
59.90	283.0
61.00	1506.0
62.00	1580.0
63.00	1251.0
64.00	256.0
65.00	411.0
68.00	3108.0
69.00	3295.0
69.90	284.0
72.00	227.0
73.00	1503.0
74.00	5294.0
75.00	15884.0
76.00	1412.0
76.90	246.0
77.80	122.0
78.90	1054.0
79.90	397.0
80.90	970.0
81.90	290.0
86.90	1313.0
87.90	1313.0
90.90	144.0
92.00	929.0
93.00	1412.0
94.00	3645.0
95.00	30712.0
96.00	2081.0
103.80	186.0
106.00	152.0
115.80	135.0
116.80	260.0
117.90	152.0
118.80	231.0
127.90	137.0
129.80	140.0
140.90	314.0
142.90	491.0
144.80	126.0
171.90	539.0
173.90	27664.0
174.90	1846.0
175.90	25696.0
176.90	1788.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

Scan 2790 (10.061 min): VV017983.D
BFB74

m/z	Abundance
39.80	184.0
43.90	307.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74