


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081518\
 Data File : VV007014.D
 Acq On : 15 Aug 2018 13:29
 Operator : SY/MD
 Sample : BFB84
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB84

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Aug 16 02:48:57 2018

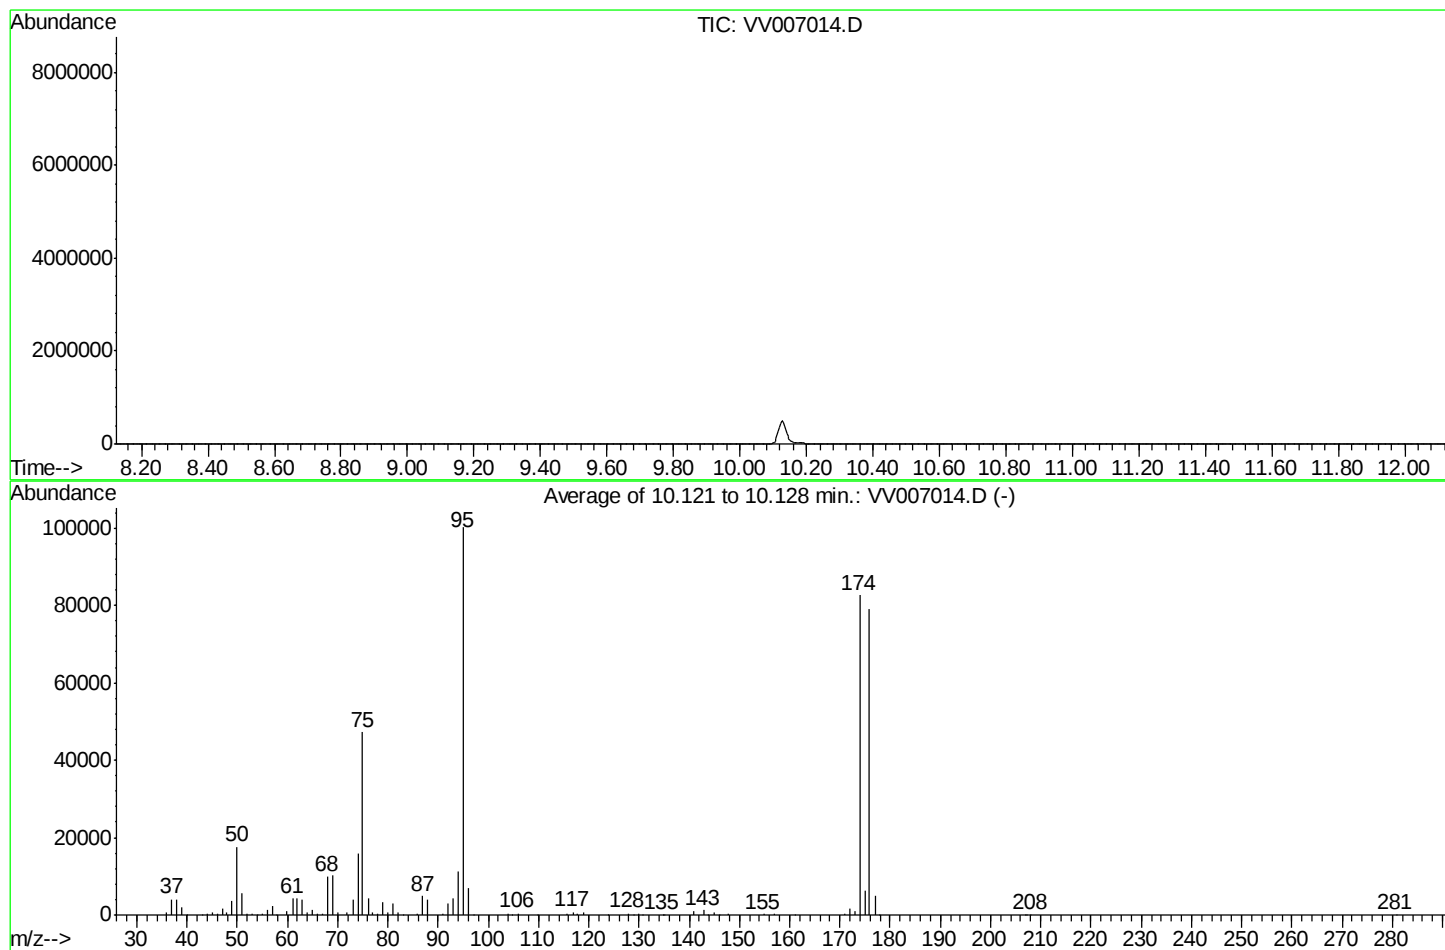

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	17633	PASS
75	95	30	80	47.1	47202	PASS
95	95	100	100	100.0	100189	PASS
96	95	5	9	7.1	7121	PASS
173	174	0.00	2	1.3	1068	PASS
174	95	50	120	82.5	82626	PASS
175	174	5	9	7.4	6143	PASS
176	174	95	101	95.7	79114	PASS
177	176	5	9	6.1	4856	PASS

Scan 2858 (10.080 min): VV007014.D
BFB84

m/z	Abundance
35.90	124.0
40.00	429.0
41.00	102.0
43.90	1193.0
206.90	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	763.0
37.00	3893.0
38.00	3682.0
39.00	1799.0
39.90	544.0
44.00	1498.0
45.00	807.0
46.00	259.0
47.00	1316.0
47.90	629.0
49.00	3574.0
50.00	16379.0
51.00	5489.0
52.10	248.0
53.00	262.0
54.10	138.0
55.00	272.0
56.00	1227.0
57.00	1966.0
57.80	104.0
59.90	862.0
61.00	3990.0
62.00	3928.0
63.00	4000.0
64.00	744.0
65.00	1263.0
66.00	181.0
67.00	283.0
68.00	9705.0
69.00	9818.0
70.00	767.0
71.80	586.0
73.00	3580.0
74.00	15306.0
75.00	44000.0
76.10	3995.0
76.90	700.0
78.00	540.0
78.90	3141.0
79.90	788.0
80.90	2724.0
82.00	759.0
85.80	179.0
86.90	4407.0
87.90	3724.0
90.90	341.0
92.00	2809.0
93.00	4069.0
94.00	10549.0
95.00	94232.0
96.00	6727.0
97.10	155.0
104.00	310.0
104.70	136.0
105.80	296.0
115.70	242.0
116.90	685.0
117.80	300.0
118.90	587.0
127.80	347.0
128.90	210.0
129.80	290.0
130.80	191.0
134.70	109.0
140.90	920.0
142.90	1159.0
144.90	471.0
145.80	104.0
147.70	185.0
154.80	296.0
156.80	180.0
170.90	229.0
171.90	1480.0
173.00	835.0
173.90	74848.0
174.90	5908.0
175.90	71584.0
176.90	4516.0
177.90	106.0
206.90	155.0
207.20	149.0
208.00	128.0
280.80	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	882.0
37.00	4135.0
38.00	4135.0
39.00	2003.0
39.90	554.0
44.00	1640.0
45.00	841.0
46.00	316.0
47.00	1561.0
47.90	696.0
49.00	3897.0
50.00	18344.0
51.00	5762.0
52.10	287.0
53.00	210.0
54.10	151.0
55.00	306.0
56.00	1322.0
57.00	2451.0
57.90	115.0
59.90	913.0
61.00	4346.0
62.00	4496.0
63.00	4206.0
64.00	717.0
65.00	1321.0
66.00	204.0
66.90	294.0
68.00	10191.0
69.00	10501.0
70.00	742.0
71.90	617.0
73.00	4022.0
74.00	16536.0
75.00	48552.0
76.10	4495.0
76.90	803.0
78.00	463.0
78.90	3407.0
79.90	830.0
80.90	3180.0
82.00	785.0
85.80	229.0
86.90	5131.0
87.90	4118.0
91.00	394.0
92.00	3090.0
93.00	4672.0
94.00	11488.0
95.00	103264.0
96.00	7315.0
97.00	159.0
104.00	317.0
104.70	137.0
105.90	404.0
115.70	224.0
116.90	751.0
117.80	359.0
118.90	649.0
127.80	372.0
128.90	143.0
129.80	318.0
130.80	175.0
134.60	129.0
140.90	1030.0
142.90	1287.0
144.90	529.0
145.90	158.0
147.80	255.0
154.80	292.0
156.80	195.0
160.90	164.0
171.00	280.0
171.90	1811.0
173.00	1099.0
173.90	85592.0
174.90	6280.0
175.90	81520.0
176.90	4905.0
177.90	131.0
206.90	177.0
208.00	122.0
280.70	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	894.0
37.00	4026.0
38.00	4110.0
39.00	1958.0
39.90	523.0
42.90	145.0
44.00	1690.0
44.90	793.0
45.90	257.0
47.00	1646.0
47.90	653.0
49.00	3848.0
50.00	18176.0
51.00	5336.0
52.00	310.0
53.00	130.0
54.10	135.0
55.00	324.0
56.00	1251.0
57.00	2724.0
57.90	108.0
60.00	842.0
61.00	4453.0
62.00	4785.0
63.00	4130.0
64.00	685.0
65.00	1325.0
66.00	163.0
66.90	301.0
68.00	9539.0
69.00	10028.0
70.00	632.0
71.90	560.0
73.00	4290.0
74.00	16075.0
75.00	49056.0
76.00	4473.0
76.90	787.0
78.90	3350.0
79.90	842.0
80.90	3254.0
81.90	723.0
83.10	119.0
85.80	217.0
86.90	5148.0
87.90	4162.0
91.00	415.0
92.00	2967.0
93.00	4666.0
94.00	11741.0
95.00	103072.0
96.00	7323.0
97.00	140.0
104.00	338.0
104.80	102.0
105.90	385.0
109.80	104.0
115.70	259.0
116.90	745.0
117.70	386.0
118.90	645.0
123.80	114.0
127.80	345.0
129.80	306.0
130.80	152.0
134.70	150.0
134.90	147.0
140.90	908.0
142.90	1345.0
143.80	130.0
144.90	572.0
146.00	192.0
147.80	304.0
154.80	264.0
156.90	180.0
160.90	187.0
171.00	279.0
171.90	2063.0
172.90	1270.0
173.90	87440.0
175.00	6242.0
175.90	84240.0
177.00	5147.0
177.90	148.0
206.80	232.0
208.00	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84