

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081519\
 Data File : VV012250.D
 Acq On : 15 Aug 2019 15:47
 Operator : SY/MD
 Sample : K4373-08
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH6

Quant Time: Aug 16 04:37:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 16 04:21:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	172289	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	165726	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	75251	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	37074	3.49	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	69.80%
7) Chloroethane-d5	1.58	69	28176	3.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	69.40%
11) 1,1-Dichloroethene-d2	2.13	63	56737	3.26	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.20%
20) 2-Butanone-d5	3.96	46	113231	49.39	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.78%
24) Chloroform-d	4.40	84	97493	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.80%
26) 1,2-Dichloroethane-d4	5.08	65	49443	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.40%
32) Benzene-d6	5.10	84	186557	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.00%
36) 1,2-Dichloropropane-d6	6.12	67	55201	4.47	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.40%
41) Toluene-d8	7.36	98	169035	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.20%
43) trans-1,3-Dichloropropene-	7.66	79	22264	4.71	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.20%
46) 2-Hexanone-d5	8.14	63	69366	45.72	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.44%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	38087	4.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	66793	5.24	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.80%


Target Compounds					Ovalue
13) Acetone	2.23	43	11896	8.327 ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081519\
Data File : VV012250.D
Acq On : 15 Aug 2019 15:47
Operator : SY/MD
Sample : K4373-08
Misc : 25mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH6

Quant Time: Aug 16 04:37:39 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 16 04:21:37 2019
Response via : Initial Calibration

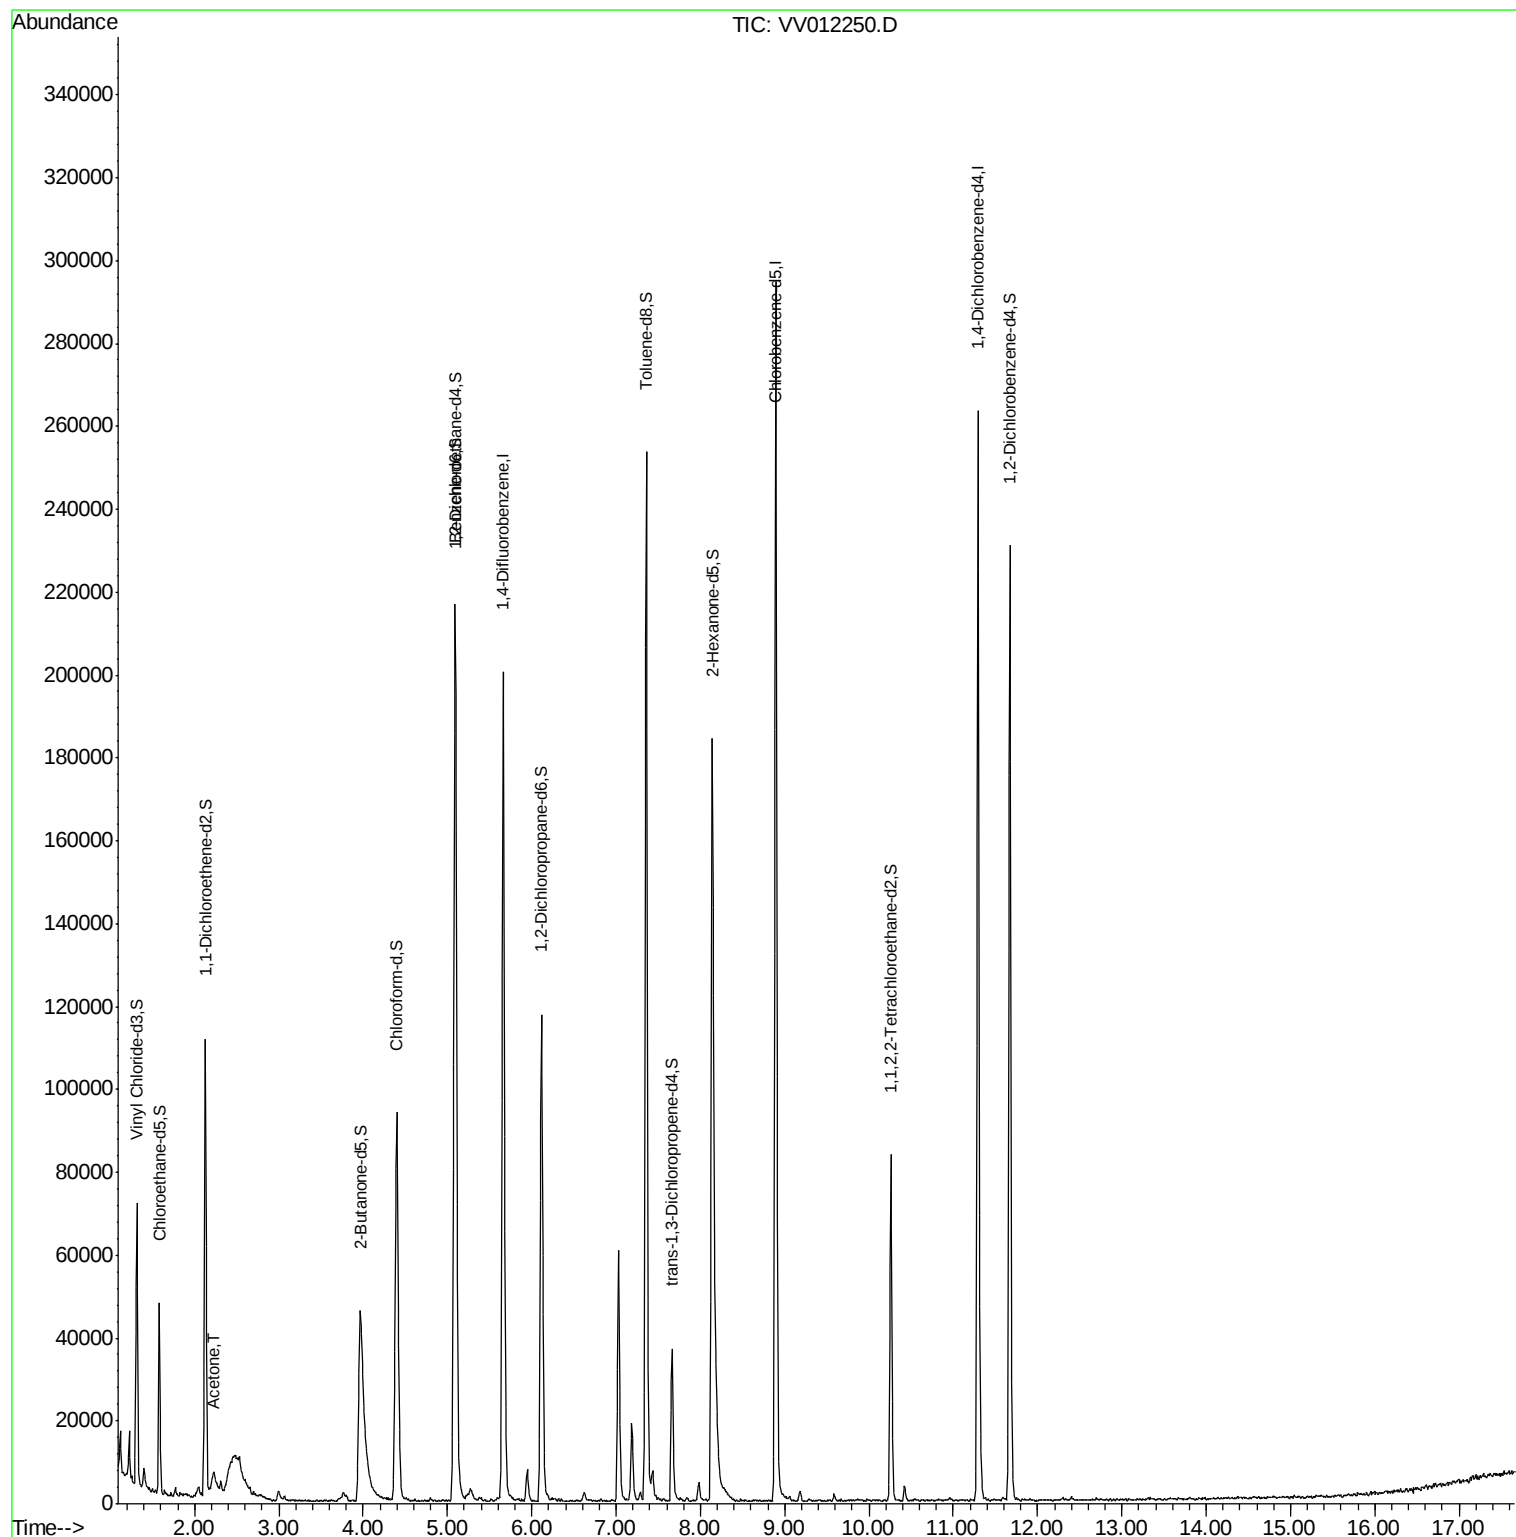

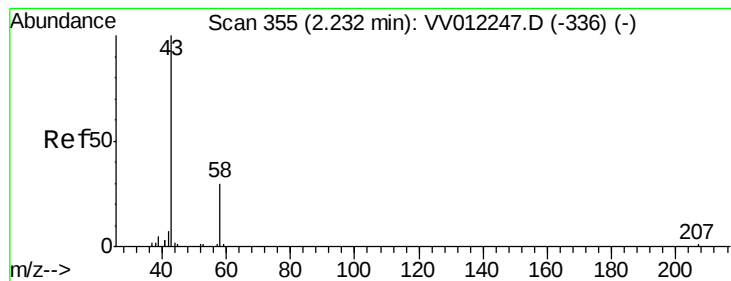

#13
 Acetone
 Concen: 8.327 ug/L
 RT: 2.23 min Scan# 354
 Delta R.T. -0.00 min
 Lab File: VV012250.D
 Acq: 15 Aug 2019 15:47

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH6

Tot Ion: 43 Resp: 11896
 Ion Ratio Lower Upper
 43 100
 58 20.8 0.0 59.4

