

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081519\
 Data File : VV012251.D
 Acq On : 15 Aug 2019 16:14
 Operator : SY/MD
 Sample : K4373-09
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ4

Quant Time: Aug 16 04:46:26 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 16 04:21:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	176054	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	173103	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	77869	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	36789	3.39	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.80%
7) Chloroethane-d5	1.58	69	26159	3.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	63.20%#
11) 1,1-Dichloroethene-d2	2.13	63	52861	2.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.60%#
20) 2-Butanone-d5	3.97	46	114162	48.73	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.46%
24) Chloroform-d	4.40	84	95669	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.00%
26) 1,2-Dichloroethane-d4	5.08	65	49338	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
32) Benzene-d6	5.09	84	185775	4.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.80%
36) 1,2-Dichloropropane-d6	6.12	67	55022	4.26	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.20%
41) Toluene-d8	7.36	98	164598	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.40%
43) trans-1,3-Dichloropropene-	7.67	79	21413	4.33	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.60%
46) 2-Hexanone-d5	8.14	63	66858	42.19	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.38%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	37952	4.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	64471	4.89	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.80%


Target Compounds					Ovalue
13) Acetone	2.22	43	7972	5.461 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081519\
Data File : VV012251.D
Acq On : 15 Aug 2019 16:14
Operator : SY/MD
Sample : K4373-09
Misc : 25mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ4

Quant Time: Aug 16 04:46:26 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 16 04:21:37 2019
Response via : Initial Calibration

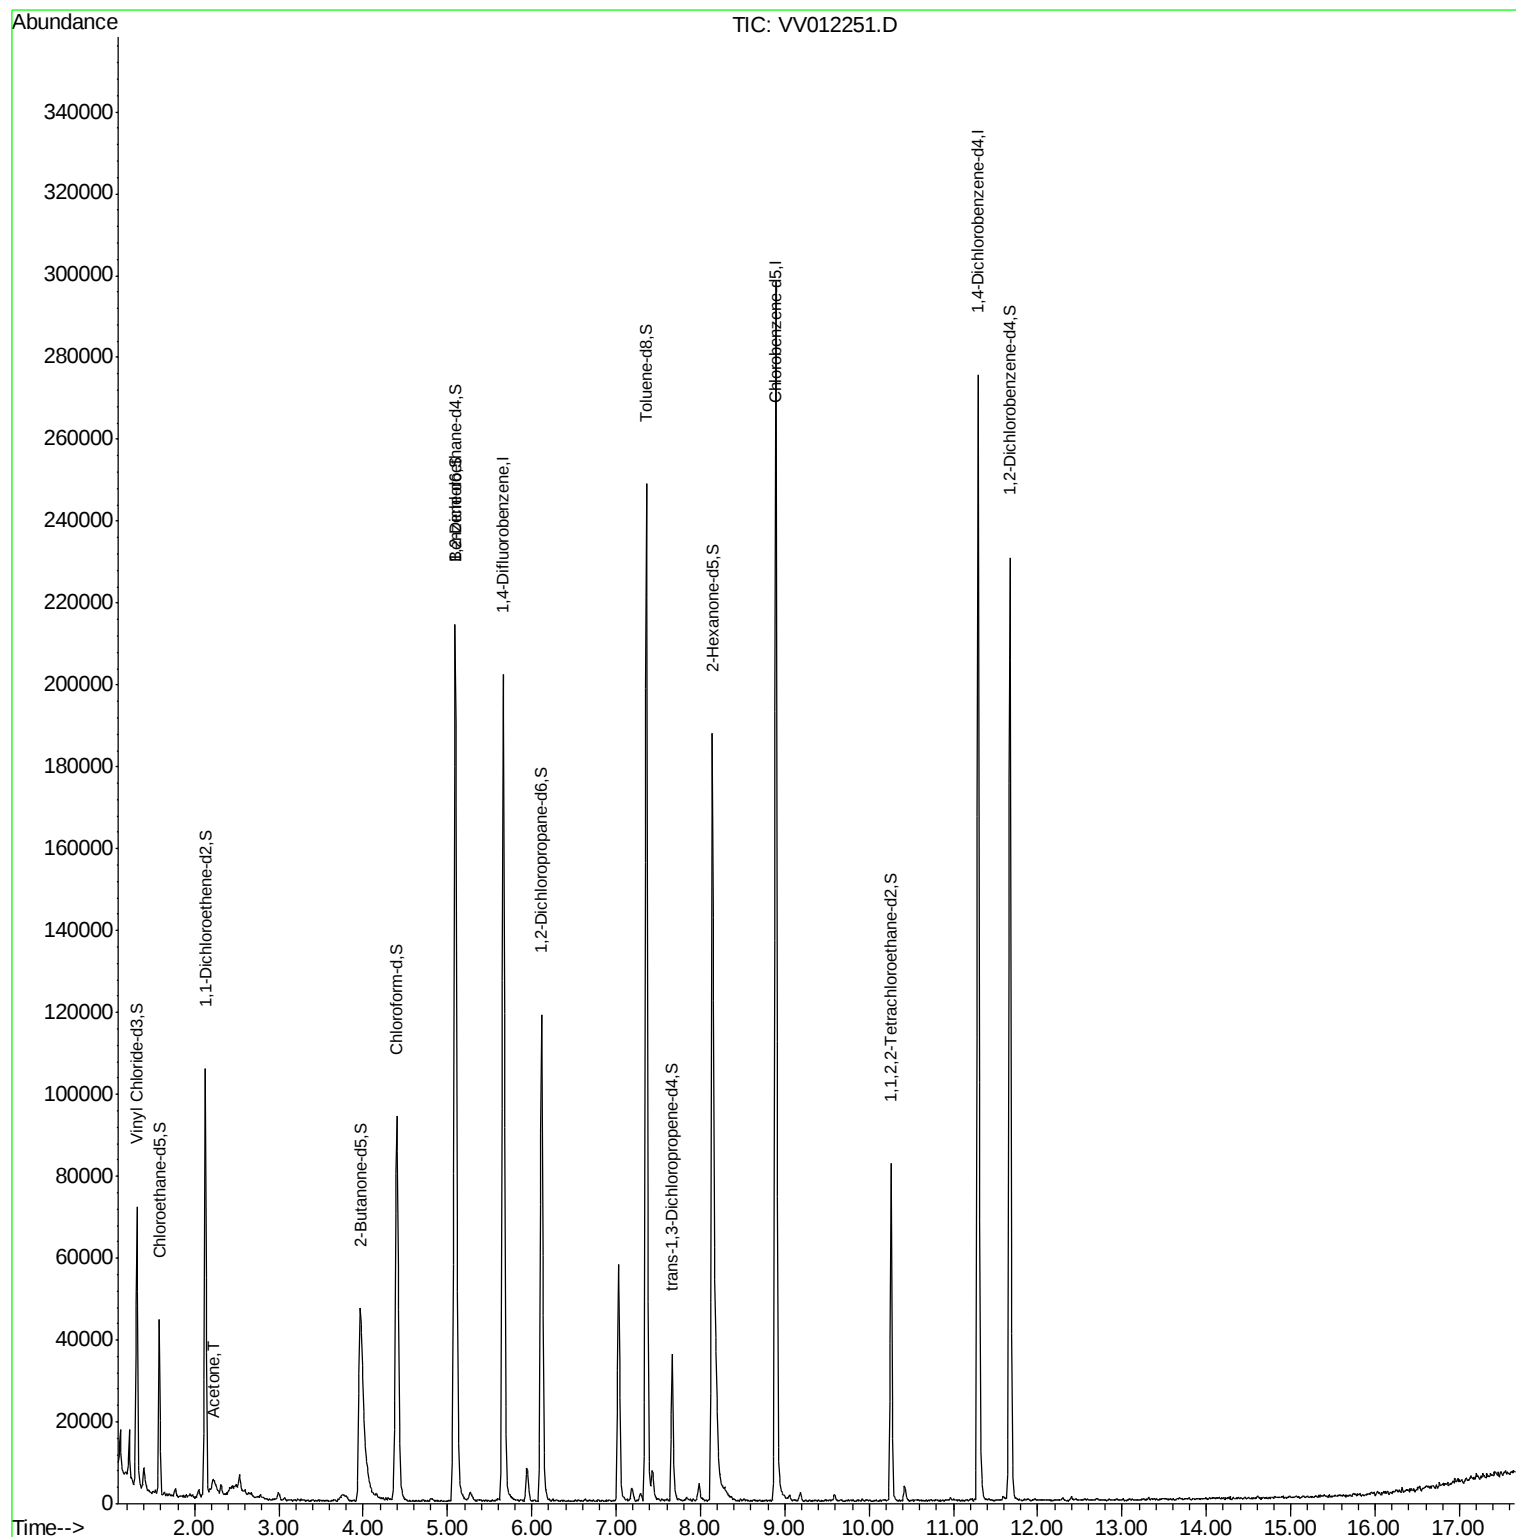

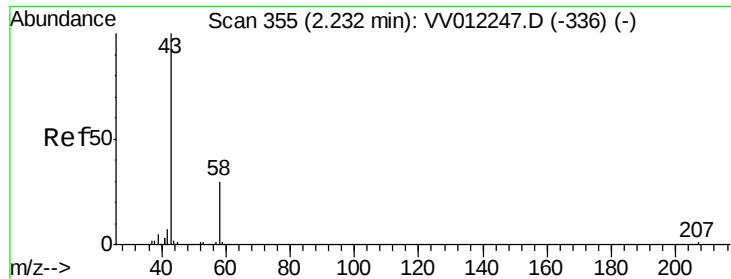

#13

Acetone

Concen: 5.461 ug/L

RT: 2.22 min Scan# 352

Delta R.T. -0.01 min

Lab File: VV012251.D

Acq: 15 Aug 2019 16:14

Instrument :

MSVOA_V

ClientSampleId :

C0AJ4

Tot Ion: 43 Resp: 7972

Ion Ratio Lower Upper

43 100

58 30.1 0.0 59.4

