

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081519\
 Data File : VV012252.D
 Acq On : 15 Aug 2019 16:42
 Operator : SY/MD
 Sample : K4373-01
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA4

Quant Time: Aug 16 04:50:12 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 16 04:21:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	155850	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	160632	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	70260	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	41252	4.30	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.00%
7) Chloroethane-d5	1.58	69	28433	3.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.40%
11) 1,1-Dichloroethene-d2	2.13	63	49936	3.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.60%
20) 2-Butanone-d5	3.93	46	86216	41.57	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.14%
24) Chloroform-d	4.40	84	89522	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
26) 1,2-Dichloroethane-d4	5.08	65	43450	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
32) Benzene-d6	5.10	84	177309	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.20%
36) 1,2-Dichloropropane-d6	6.12	67	51602	4.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.20%
41) Toluene-d8	7.36	98	162879	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.80%
43) trans-1,3-Dichloropropene-	7.66	79	20048	4.37	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.40%
46) 2-Hexanone-d5	8.13	63	61612	41.90	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.80%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	37933	4.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	65879	5.54	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.80%


Target Compounds					Ovalue
13) Acetone	2.19	43	3569	2.762 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081519\
Data File : VV012252.D
Acq On : 15 Aug 2019 16:42
Operator : SY/MD
Sample : K4373-01
Misc : 25mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA4

Quant Time: Aug 16 04:50:12 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 16 04:21:37 2019
Response via : Initial Calibration

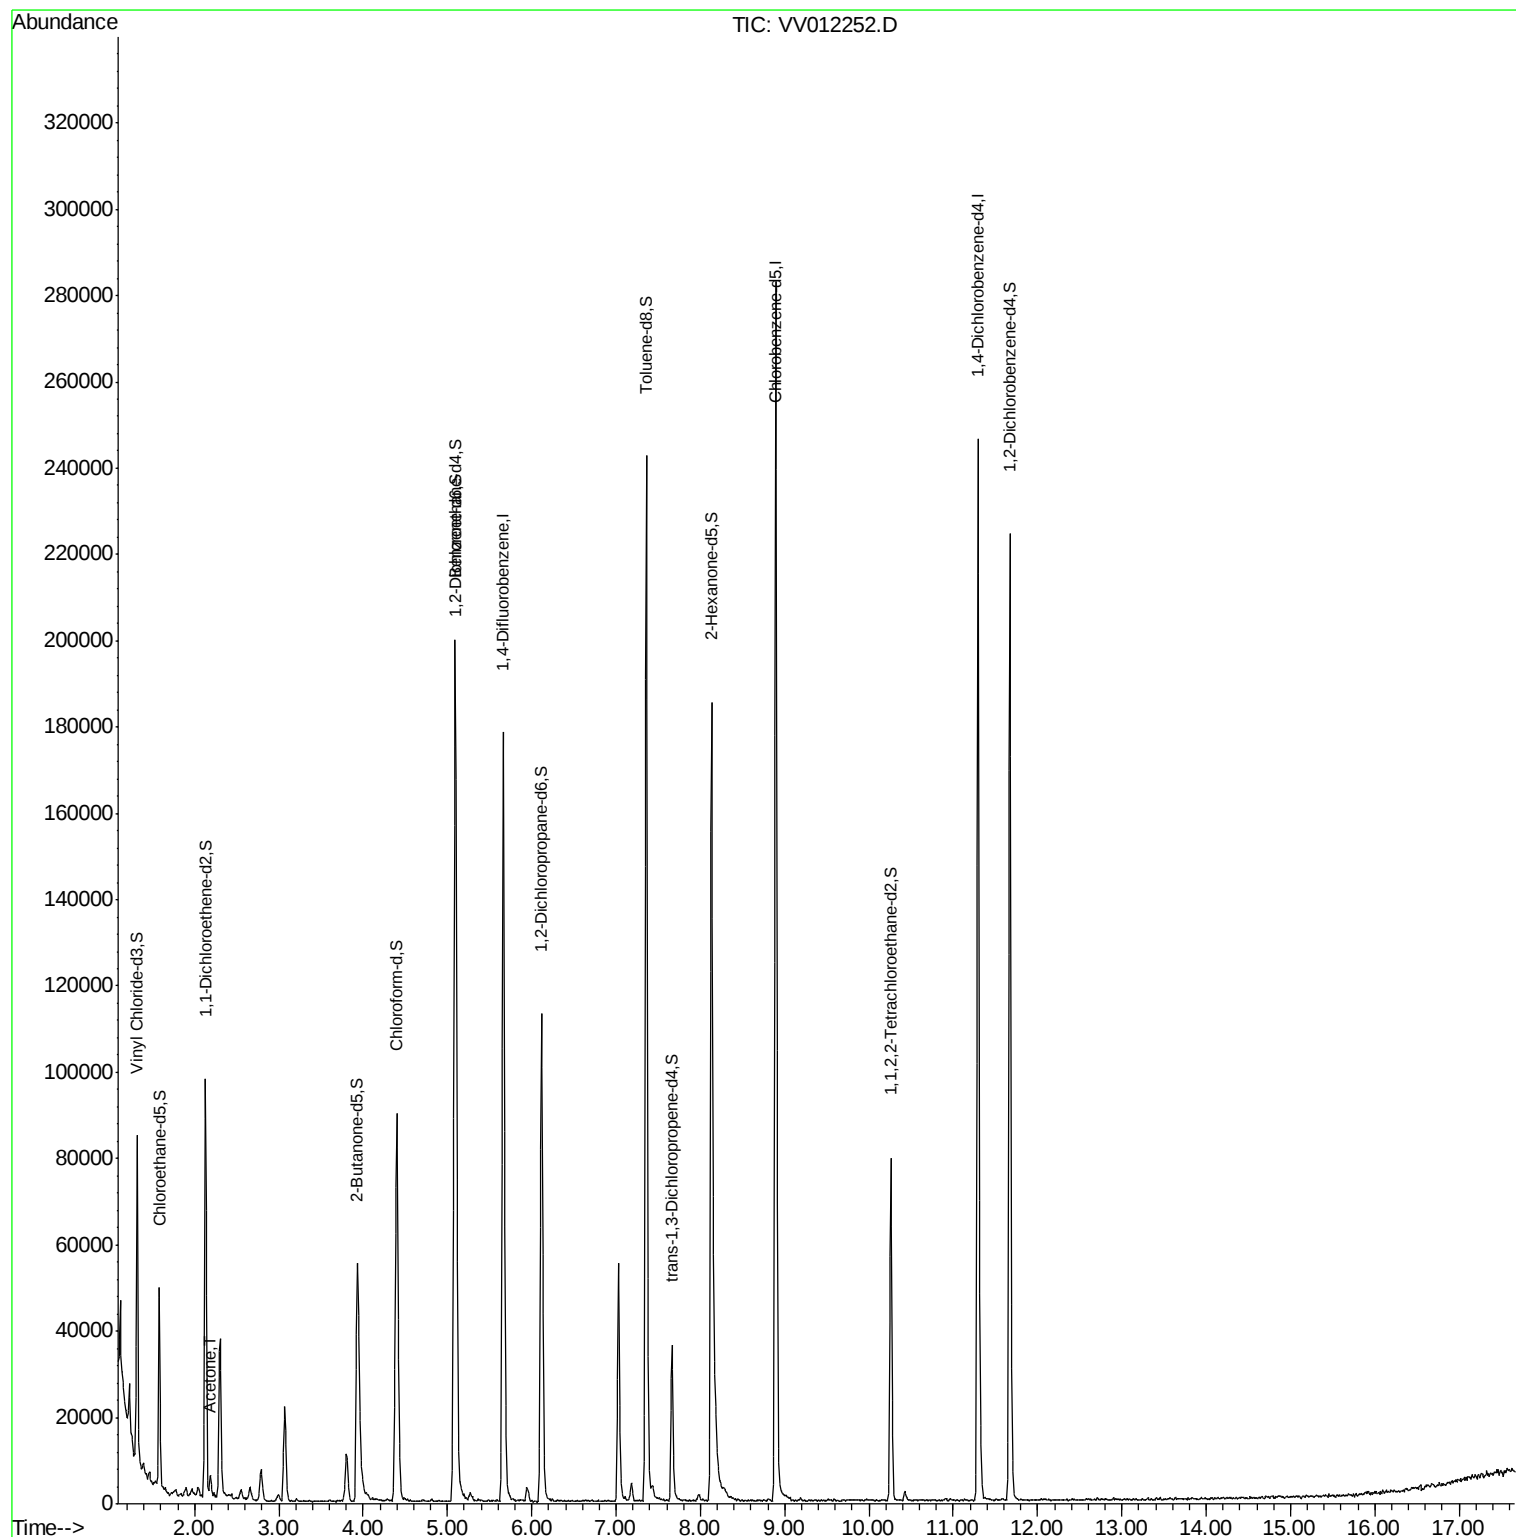

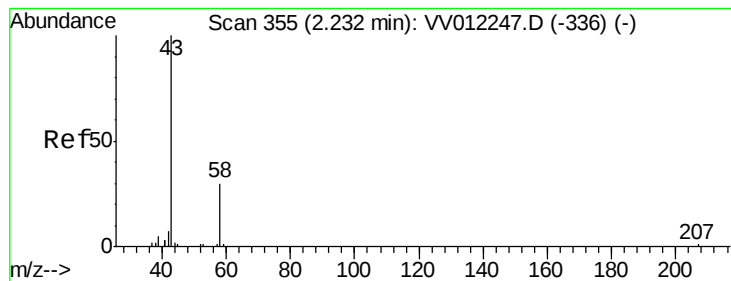

#13

Acetone

Concen: 2.762 ug/L

RT: 2.19 min Scan# 341

Delta R.T. -0.05 min

Lab File: VV012252.D

Acq: 15 Aug 2019 16:42

Instrument :
MSVOA_V
ClientSampleId :
C0AA4

Tot Ion: 43 Resp: 3569

Ion Ratio Lower Upper

43 100

58 21.8 0.0 59.4

