

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081519\
 Data File : VV012254.D
 Acq On : 15 Aug 2019 17:37
 Operator : SY/MD
 Sample : K4373-04
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC0

Quant Time: Aug 16 05:00:32 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 16 04:21:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	149643	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	145720	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	64663	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	44029	4.77	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.40%
7) Chloroethane-d5	1.58	69	28574	4.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.20%
11) 1,1-Dichloroethene-d2	2.13	63	50852	3.37	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.40%
20) 2-Butanone-d5	3.94	46	40550	20.36	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	40.72%
24) Chloroform-d	4.40	84	82861	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.80%
26) 1,2-Dichloroethane-d4	5.08	65	46201	5.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.00%
32) Benzene-d6	5.10	84	166744	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
36) 1,2-Dichloropropane-d6	6.12	67	48123	4.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.60%
41) Toluene-d8	7.36	98	150263	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.20%
43) trans-1,3-Dichloropropene-	7.66	79	18834	4.53	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.60%
46) 2-Hexanone-d5	8.13	63	52923	39.67	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.34%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	34206	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	59703	5.45	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.00%


Target Compounds					Ovalue
13) Acetone	2.19	43	3784	3.049 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081519\
Data File : VV012254.D
Acq On : 15 Aug 2019 17:37
Operator : SY/MD
Sample : K4373-04
Misc : 25mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC0

Quant Time: Aug 16 05:00:32 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 16 04:21:37 2019
Response via : Initial Calibration

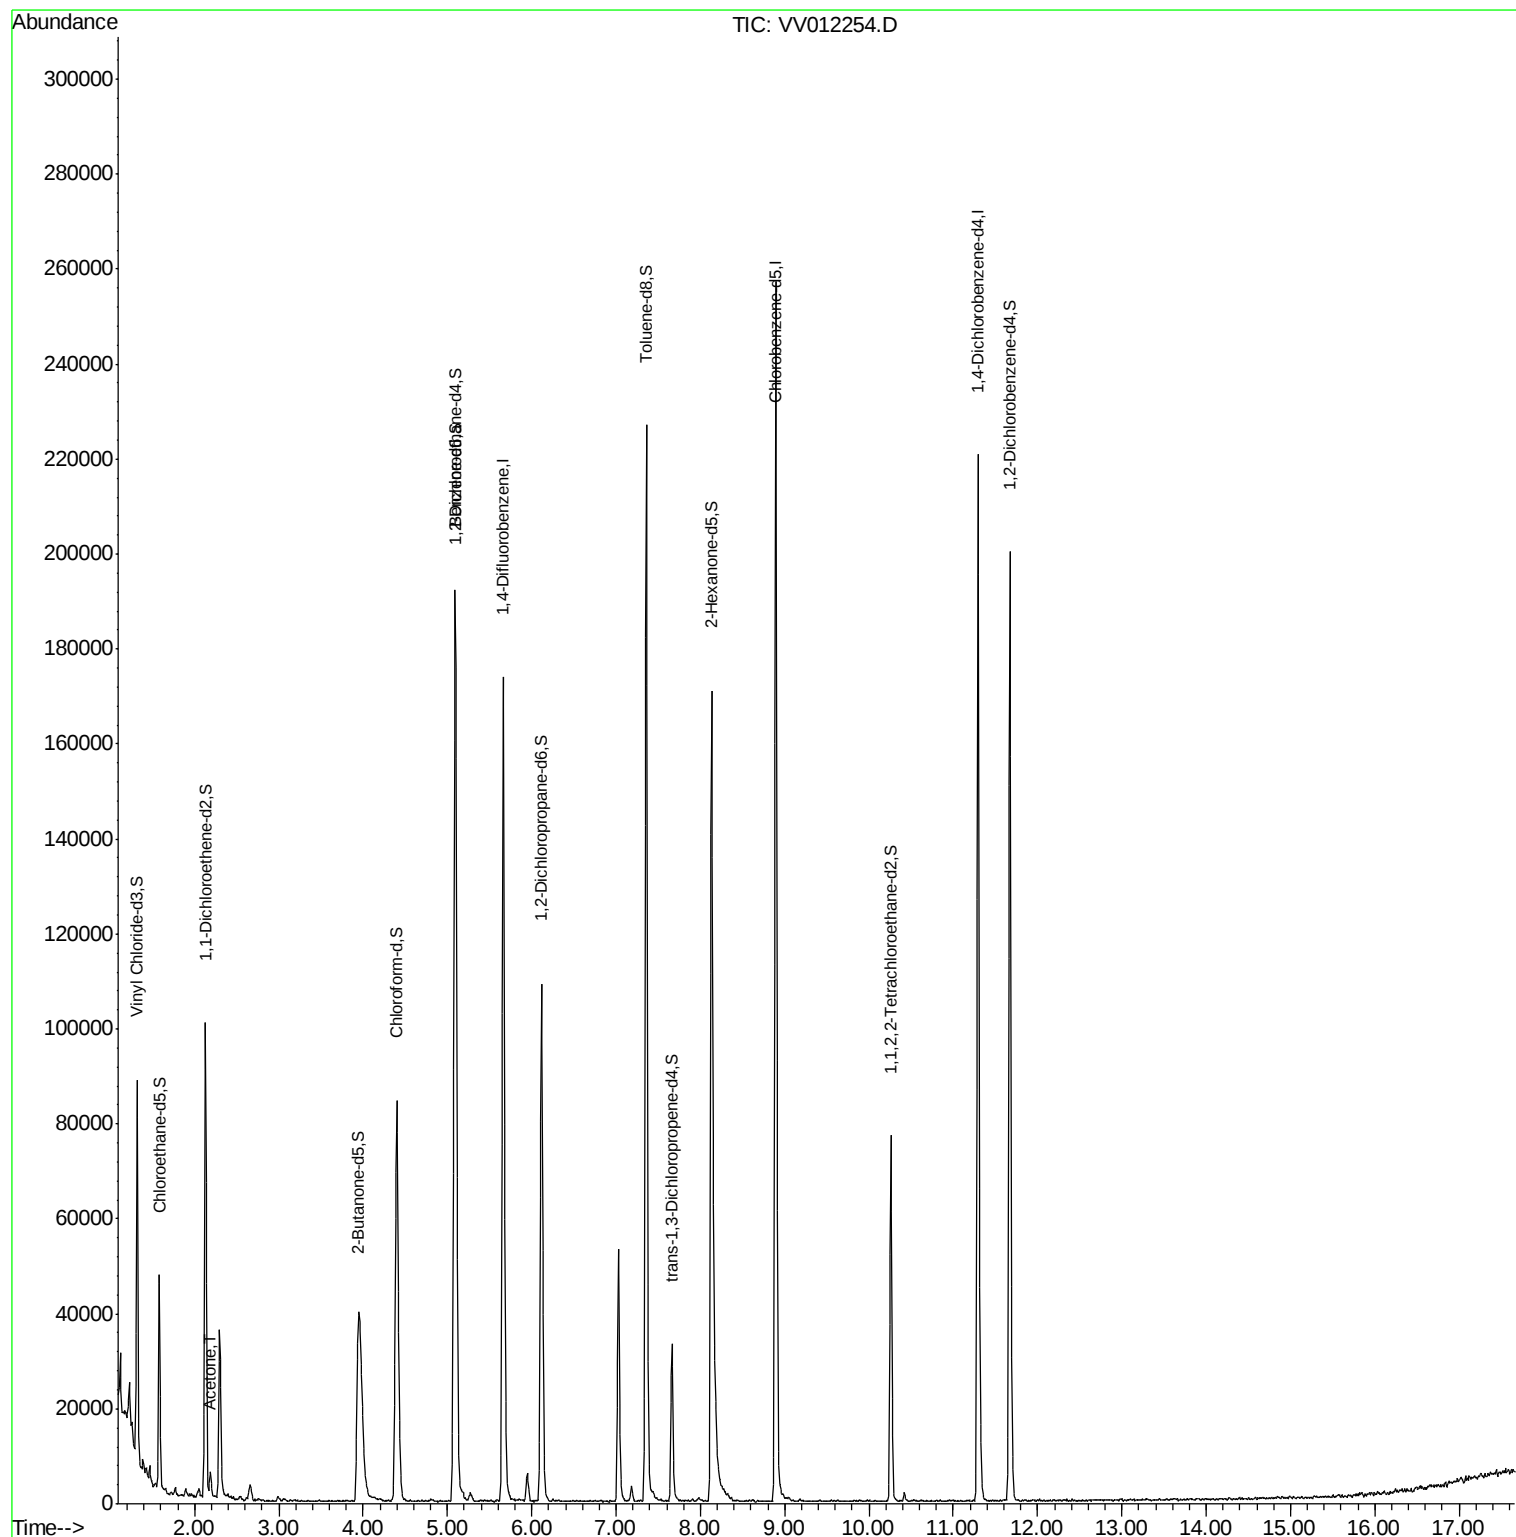

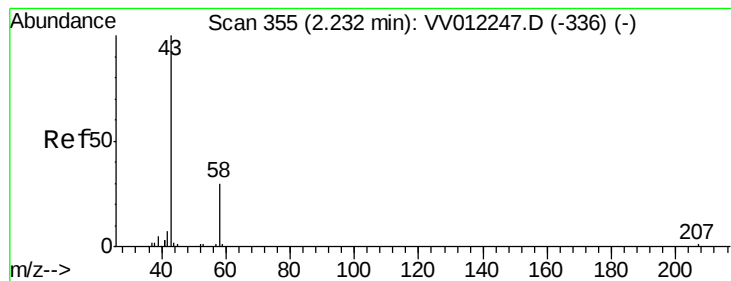

#13

Acetone

Concen: 3.049 ug/L

RT: 2.19 min Scan# 341

Delta R.T. -0.04 min

Lab File: VV012254.D

Acq: 15 Aug 2019 17:37

Instrument :
MSVOA_V
ClientSampleId :
C0AC0

Tot Ion: 43 Resp: 3784

Ion Ratio Lower Upper

43 100

58 26.9 0.0 59.4

