

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081519\
 Data File : VV012257.D
 Acq On : 15 Aug 2019 19:00
 Operator : SY/MD
 Sample : K4337-20
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB8

Quant Time: Aug 16 05:09:42 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 16 04:21:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	152105	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	150097	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	71068	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	39006	4.16	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.20%
7) Chloroethane-d5	1.58	69	28634	4.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.00%
11) 1,1-Dichloroethene-d2	2.13	63	52310	3.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.20%
20) 2-Butanone-d5	3.93	46	65527	32.38	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	64.76%
24) Chloroform-d	4.40	84	85385	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.00%
26) 1,2-Dichloroethane-d4	5.08	65	45964	5.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.60%
32) Benzene-d6	5.10	84	169064	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.00%
36) 1,2-Dichloropropane-d6	6.12	67	48379	4.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.40%
41) Toluene-d8	7.36	98	157987	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.20%
43) trans-1,3-Dichloropropene-	7.66	79	19731	4.61	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.20%
46) 2-Hexanone-d5	8.13	63	60019	43.68	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.36%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	35733	4.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	66451	5.52	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.40%


Target Compounds					Ovalue
13) Acetone	2.18	43	4030	3.195 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081519\
Data File : VV012257.D
Acq On : 15 Aug 2019 19:00
Operator : SY/MD
Sample : K4337-20
Misc : 25mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB8

Quant Time: Aug 16 05:09:42 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 16 04:21:37 2019
Response via : Initial Calibration

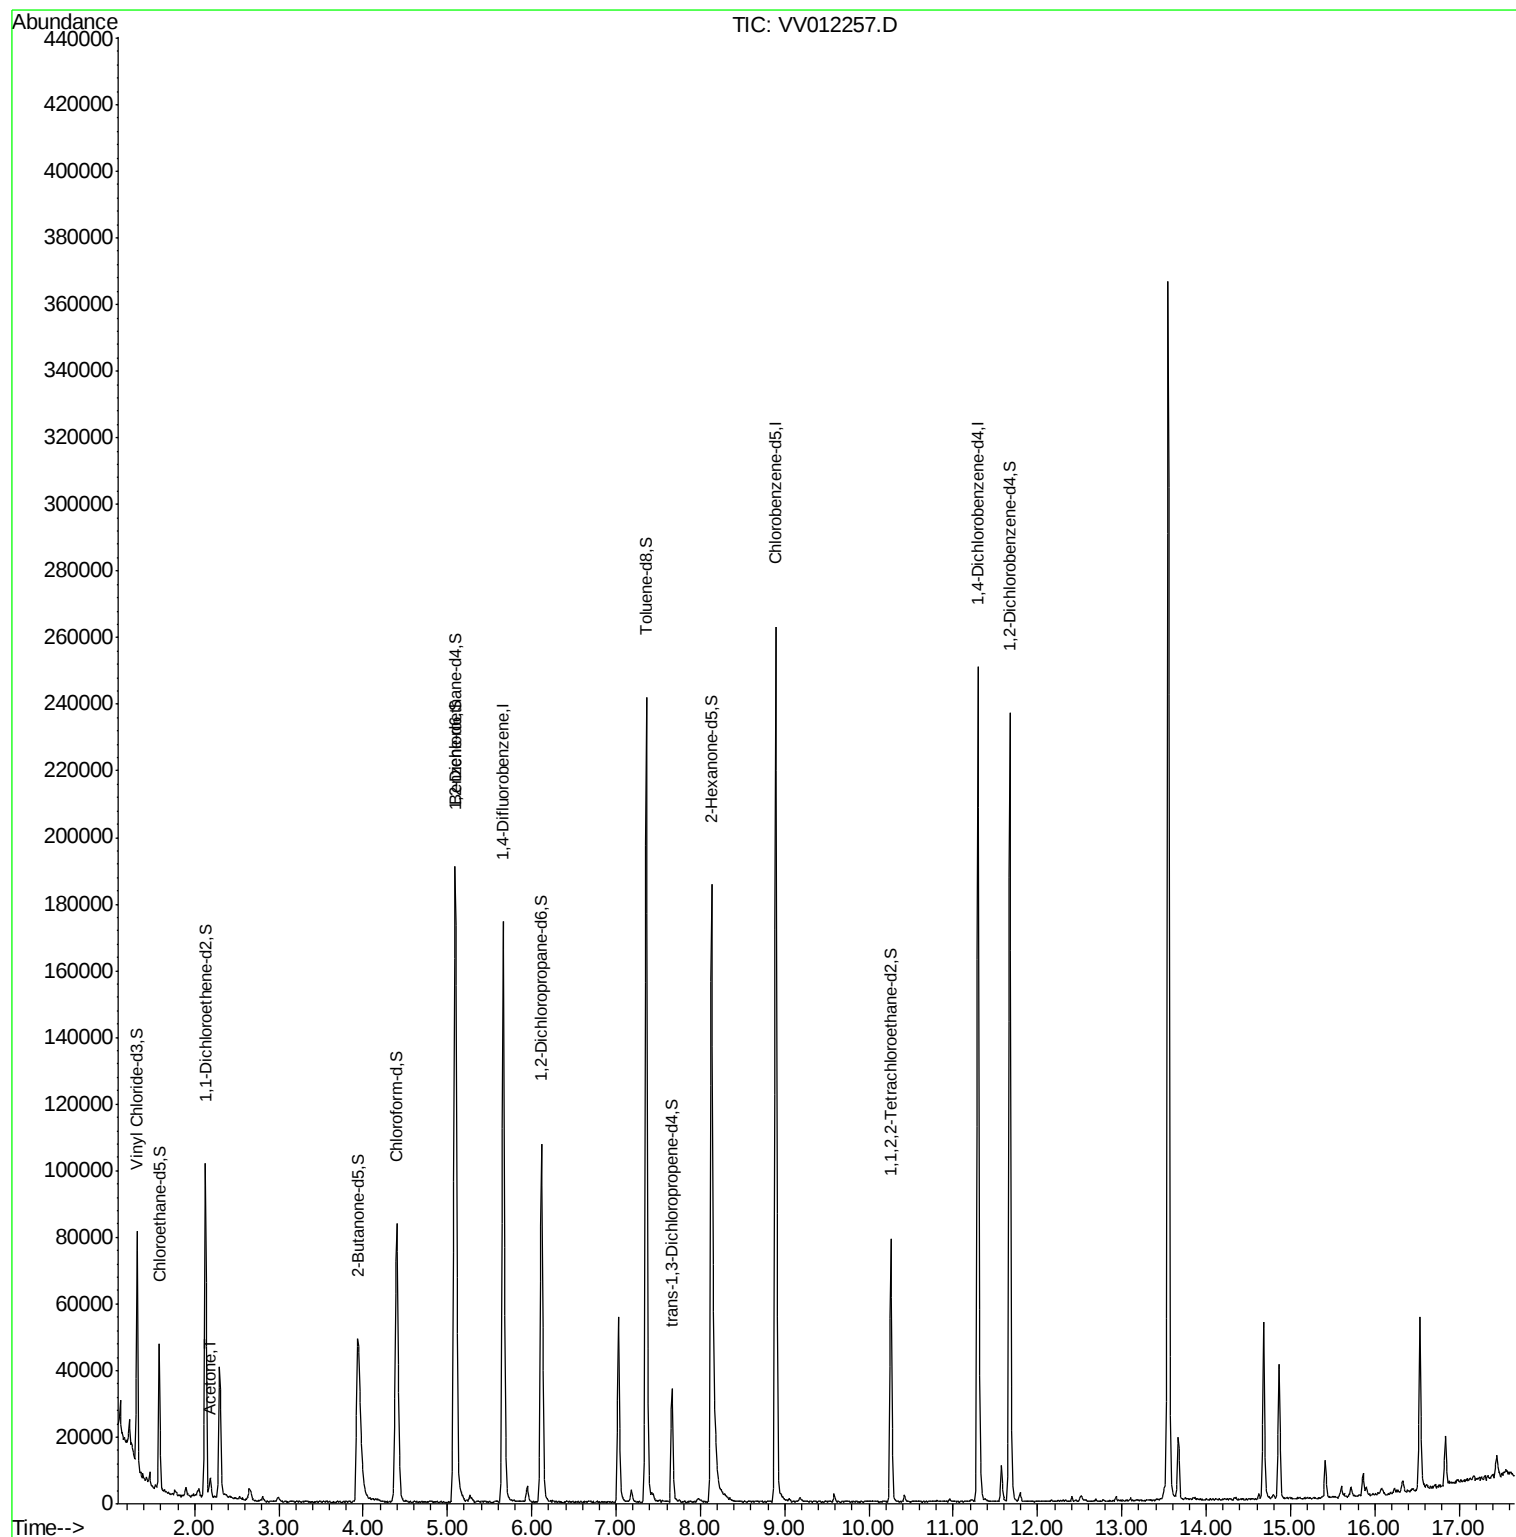

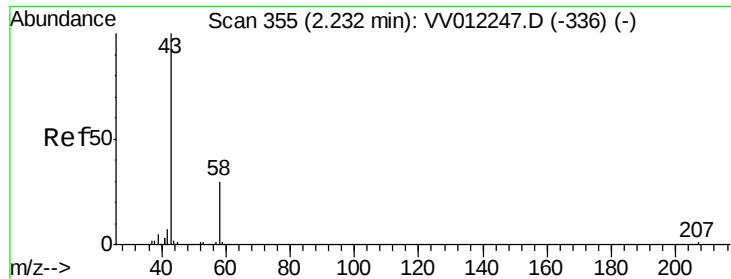

#13

Acetone

Concen: 3.195 ug/L

RT: 2.18 min Scan# 340

Delta R.T. -0.05 min

Lab File: VV012257.D

Acq: 15 Aug 2019 19:00

Instrument :

MSVOA_V

ClientSampleId :

C0AB8

Tot Ion: 43 Resp: 4030

Ion Ratio Lower Upper

43 100

58 29.6 0.0 59.4

