

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081519\
 Data File : VV012253.D
 Acq On : 15 Aug 2019 17:09
 Operator : SY/MD
 Sample : K4373-02
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.225	39	42	47	rVB2	7266	5984	1.13%	0.129%
2	1.319	63	71	83	rVB	76739	85636	16.18%	1.850%
3	1.582	145	153	165	rVB	48158	55413	10.47%	1.197%
4	2.129	311	323	333	rBV	116039	165898	31.35%	3.584%
5	2.187	336	341	349	rVB5	5054	6927	1.31%	0.150%
6	2.299	366	376	390	rBV	15327	28731	5.43%	0.621%
7	2.804	519	533	552	rBV3	54783	113226	21.40%	2.446%
8	3.978	872	898	928	rBV9	36624	170909	32.30%	3.692%
9	4.399	1012	1029	1057	rBV2	87357	231649	43.78%	5.004%
10	5.093	1227	1245	1275	rBV2	216850	529154	100.00%	11.431%
11	5.334	1313	1320	1332	rVB6	3951	7576	1.43%	0.164%
12	5.662	1405	1422	1444	rBV	195297	387334	73.20%	8.367%
13	5.958	1499	1514	1528	rVB9	15205	35231	6.66%	0.761%
14	6.116	1549	1563	1580	rBV	120806	245098	46.32%	5.295%
15	7.029	1835	1847	1868	rBV	58621	106455	20.12%	2.300%
16	7.357	1936	1949	1964	rBV	254613	442148	83.56%	9.551%
17	7.666	2034	2045	2064	rBV2	34380	59258	11.20%	1.280%
18	8.016	2145	2154	2170	rVB3	14947	25479	4.82%	0.550%
19	8.135	2179	2191	2233	rBV3	163616	404657	76.47%	8.742%
20	8.894	2415	2427	2448	rBV	292549	482952	91.27%	10.433%
21	9.974	2752	2763	2774	rBV2	15387	23823	4.50%	0.515%
22	10.260	2835	2852	2871	rBV	78863	127270	24.05%	2.749%
23	11.292	3161	3173	3198	rBV	249002	423163	79.97%	9.141%
24	11.572	3249	3260	3272	rBV2	38023	61384	11.60%	1.326%
25	11.672	3278	3291	3311	rBV	230453	388719	73.46%	8.397%
26	12.161	3436	3443	3452	rVB4	5752	7563	1.43%	0.163%
27	12.929	3675	3682	3692	rVB5	4859	7475	1.41%	0.161%


Sum of corrected areas: 4629112

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081519\
Data File : VV012253.D
Acq On : 15 Aug 2019 17:09
Operator : SY/MD
Sample : K4373-02
Misc : 25mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0AA8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

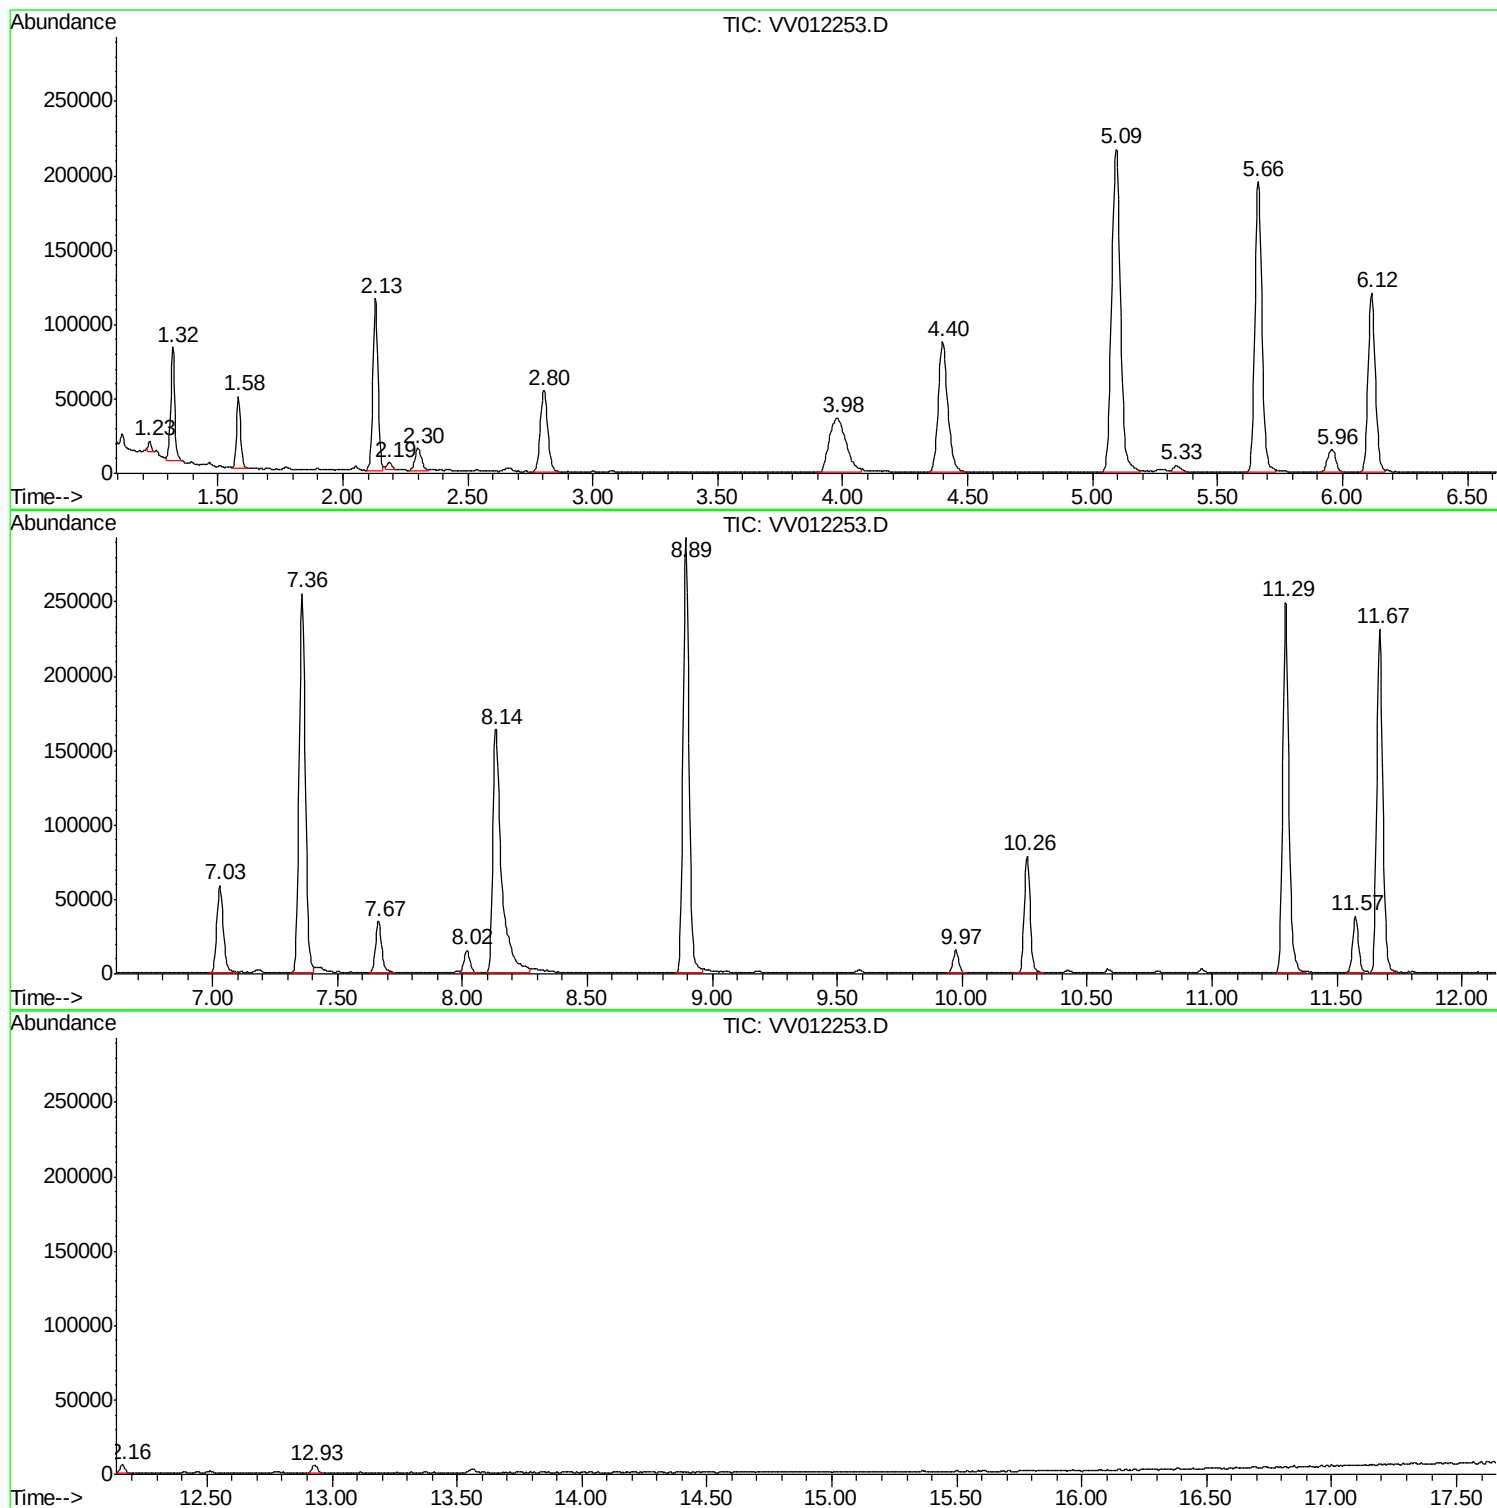

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081519\
Data File : VV012253.D
Acq On : 15 Aug 2019 17:09
Operator : SY/MD
Sample : K4373-02
Misc : 25mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA8










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Indane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.57	0.73 ug/L	61384	1,4-Dichlorobenzene-d4	11.29

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Indane		118	C9H10	000496-11-7	93
2	trans-Cinnamyl bromide		196	C9H9Br	026146-77-0	59
3	7-Methylenecycloocta-1,3,5-triene		118	C9H10	002570-13-0	53
4	Indane		118	C9H10	000496-11-7	50
5	Indane		118	C9H10	000496-11-7	50

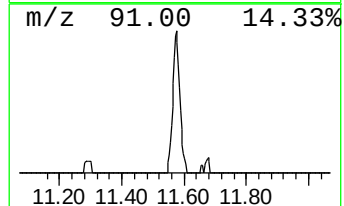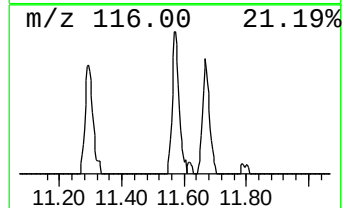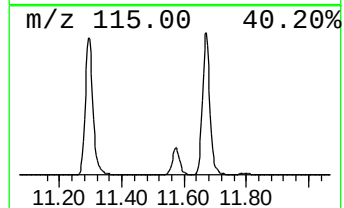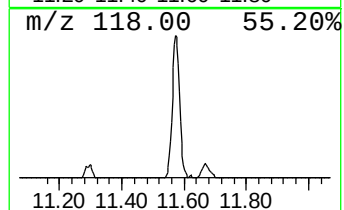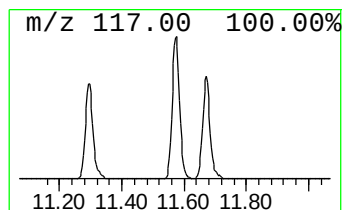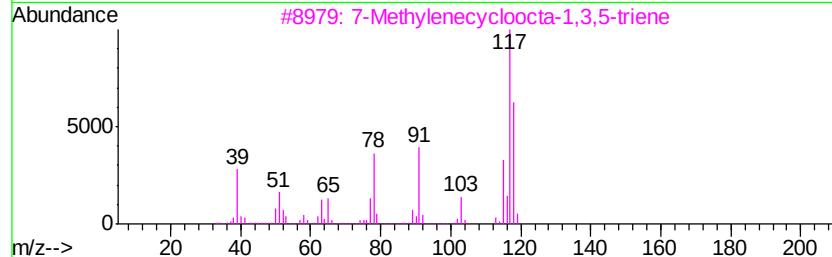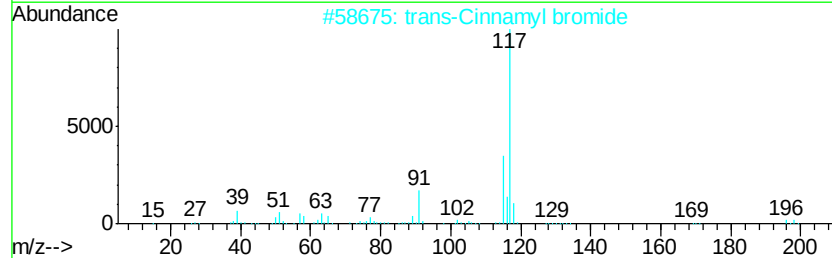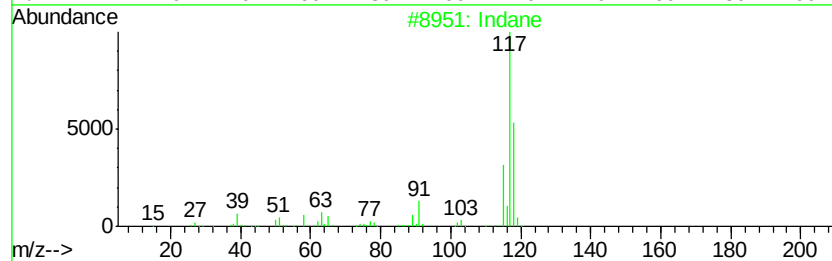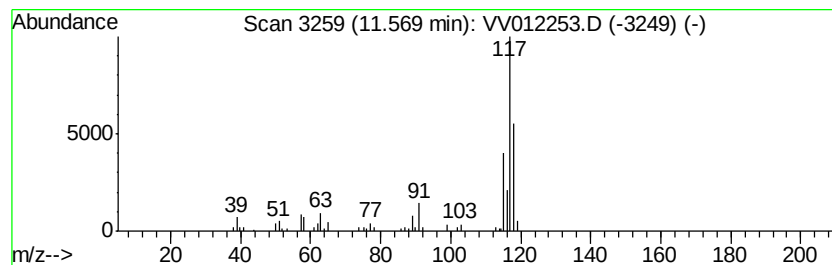

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081519\
Data File : VV012253.D
Acq On : 15 Aug 2019 17:09
Operator : SY/MD
Sample : K4373-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	11.57	0.7	ug/L	61384	3	11.29	423163	5.0