

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081519\
 Data File : VV012259.D
 Acq On : 15 Aug 2019 20:22
 Operator : SY/MD
 Sample : K4373-06 50X
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.116	5	8	21	rVB2	9564	10232	1.83%	0.215%
2	1.225	39	42	47	rVB	9689	7865	1.40%	0.166%
3	1.315	62	70	79	rBV	67522	73348	13.09%	1.544%
4	1.582	145	153	165	rVB	53507	59335	10.59%	1.249%
5	2.129	313	323	334	rBV	121785	171472	30.60%	3.609%
6	2.534	441	449	456	rBV4	3845	5928	1.06%	0.125%
7	3.962	875	893	935	rBV2	58011	217207	38.77%	4.571%
8	4.399	1012	1029	1054	rBV	101744	252350	45.04%	5.311%
9	5.093	1228	1245	1266	rBV2	236178	560293	100.00%	11.791%
10	5.662	1408	1422	1440	rBV	211687	418059	74.61%	8.798%
11	5.945	1499	1510	1525	rBV6	5080	10331	1.84%	0.217%
12	6.116	1548	1563	1587	rBV	128856	262925	46.93%	5.533%
13	7.029	1833	1847	1867	rBV	64786	118493	21.15%	2.494%
14	7.357	1935	1949	1967	rBV	268444	470425	83.96%	9.900%
15	7.662	2034	2044	2064	rBV	38869	69269	12.36%	1.458%
16	8.142	2181	2193	2230	rBV2	214311	506693	90.43%	10.663%
17	8.894	2415	2427	2455	rBV	296895	499995	89.24%	10.523%
18	10.260	2840	2852	2868	rBV	93157	148435	26.49%	3.124%
19	11.293	3159	3173	3198	rBV	280289	455439	81.29%	9.585%
20	11.669	3279	3290	3311	rBV	250238	409230	73.04%	8.612%
21	13.553	3866	3876	3889	rBV	14746	24350	4.35%	0.512%


Sum of corrected areas: 4751674

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081519\
Data File : VV012259.D
Acq On : 15 Aug 2019 20:22
Operator : SY/MD
Sample : K4373-06 50X
Misc : 25mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

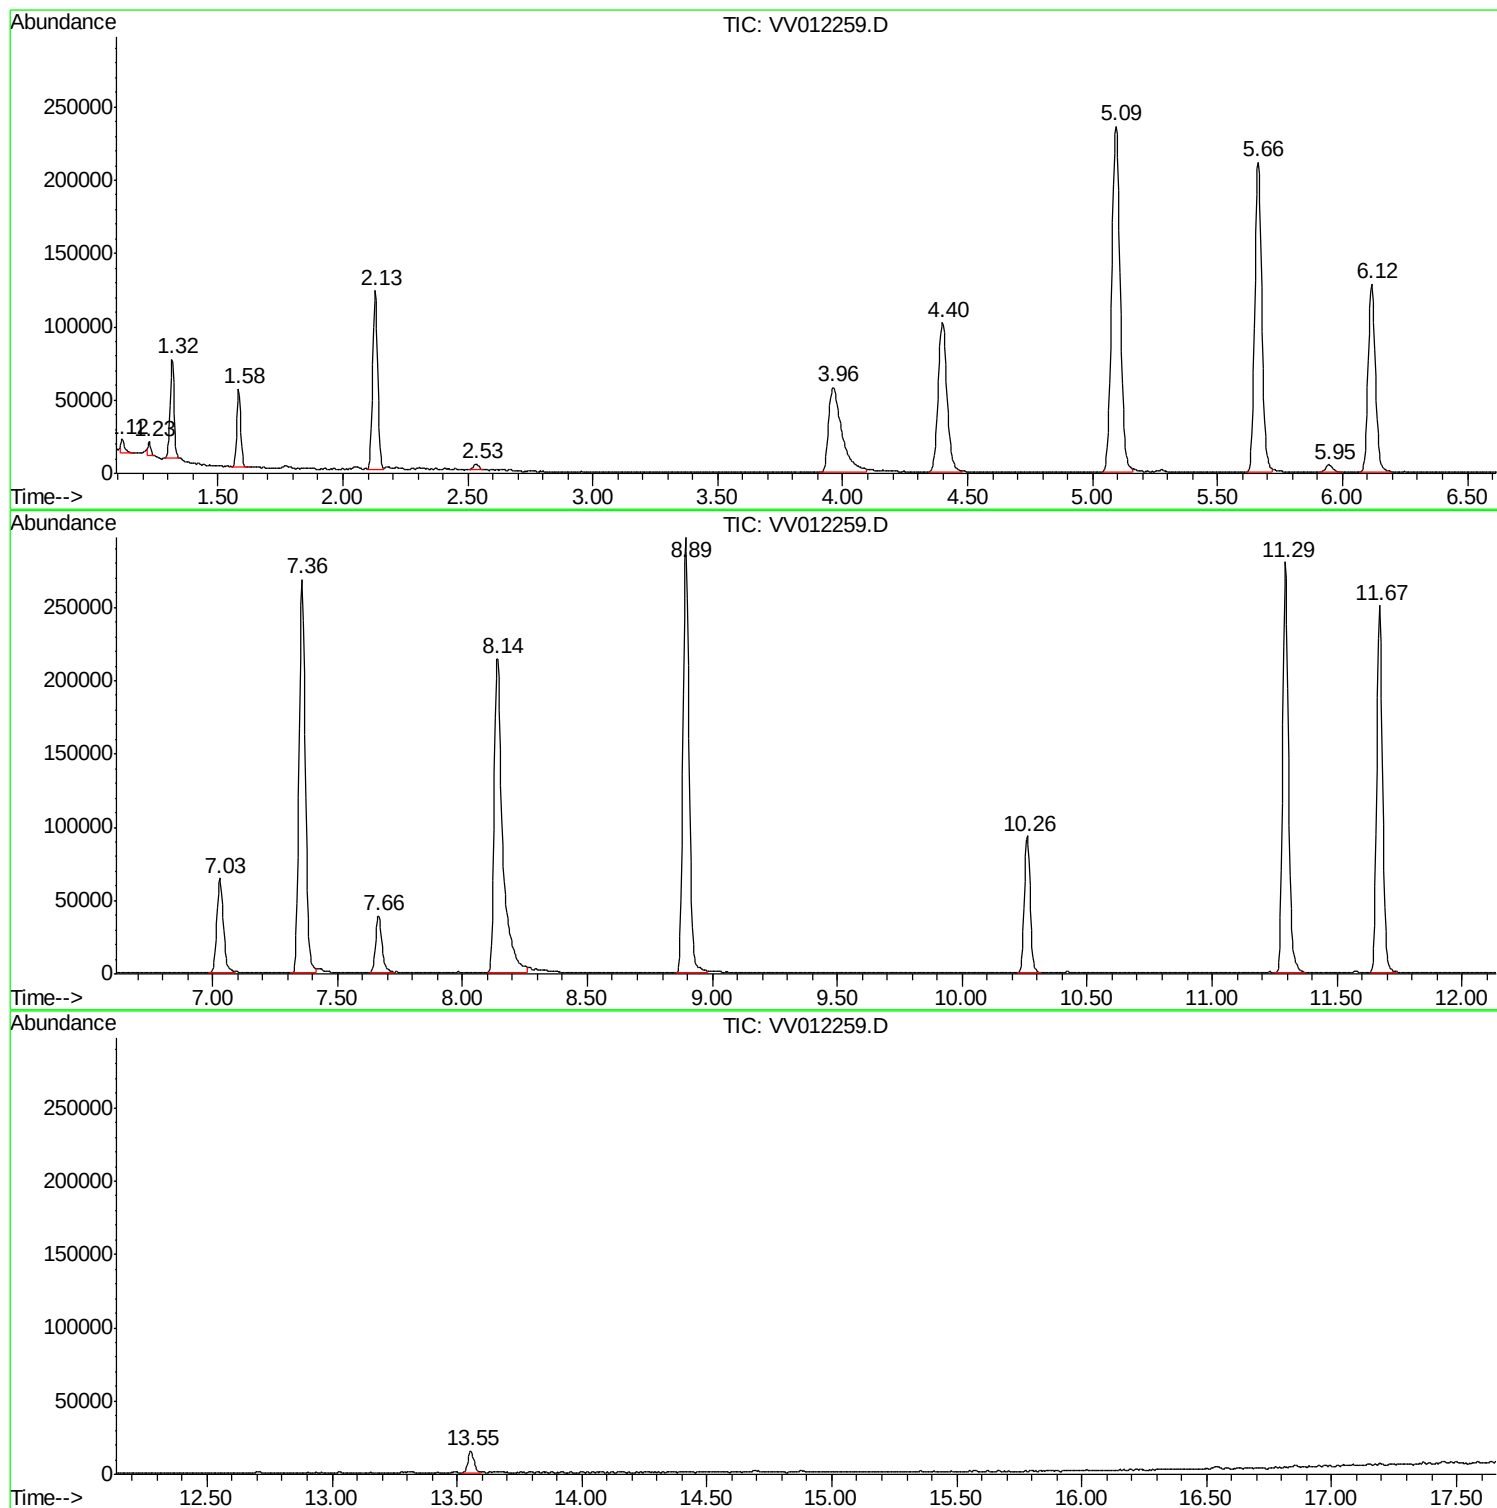

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081519\
Data File : VV012259.D
Acq On : 15 Aug 2019 20:22
Operator : SY/MD
Sample : K4373-06 50X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081519\
Data File : VV012259.D
Acq On : 15 Aug 2019 20:22
Operator : SY/MD
Sample : K4373-06 50X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc