


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081519\
Data File : VV012246.D
Acq On : 15 Aug 2019 11:00
Operator : SY/MD
Sample : BFB48
Misc : 25mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB48

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Aug 16 10:50:59 2019

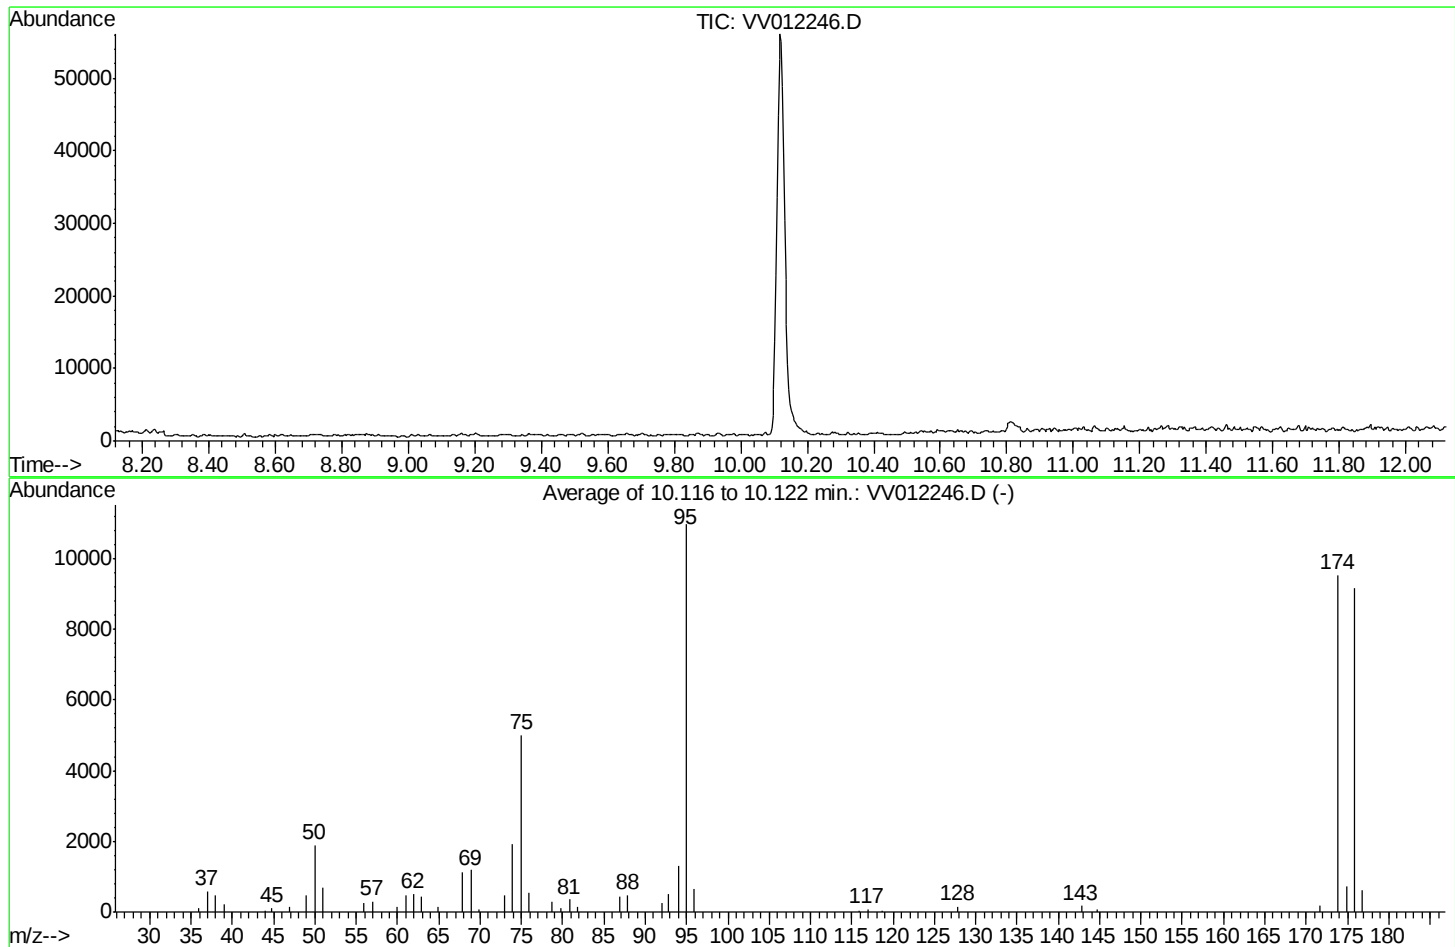

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	1899	PASS
75	95	30	80	45.7	5010	PASS
95	95	100	100	100.0	10969	PASS
96	95	5	9	6.1	669	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.8	9526	PASS
175	174	5	9	7.7	735	PASS
176	174	95	101	96.1	9153	PASS
177	176	5	9	6.8	618	PASS

m/z	Abundance
35.90	112.0
37.00	623.0
37.90	398.0
38.90	216.0
39.90	411.0
43.90	507.0
44.80	142.0
46.90	129.0
49.00	497.0
50.00	1792.0
50.90	691.0
55.90	196.0
57.00	297.0
59.90	143.0
61.00	468.0
62.00	561.0
62.90	393.0
64.90	143.0
67.90	1258.0
68.90	1175.0
69.80	102.0
73.00	513.0
74.00	1781.0
75.00	4779.0
76.00	582.0
78.70	295.0
79.80	112.0
80.90	362.0
81.70	149.0
86.80	397.0
87.90	508.0
91.90	253.0
92.80	499.0
94.00	1207.0
95.00	10715.0
96.00	687.0
115.80	117.0
127.90	162.0
142.80	132.0
171.70	159.0
173.90	8997.0
174.90	676.0
175.90	8694.0
176.80	620.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
35.80	126.0
37.00	612.0
37.90	502.0
39.00	213.0
39.90	478.0
43.90	380.0
44.80	127.0
46.90	151.0
48.90	505.0
50.00	1943.0
50.90	694.0
55.90	264.0
57.00	316.0
59.90	185.0
61.00	483.0
61.90	534.0
62.80	458.0
64.90	150.0
67.90	1178.0
68.90	1240.0
73.00	485.0
73.90	2009.0
75.00	5151.0
75.90	565.0
78.70	292.0
79.80	123.0
80.80	353.0
81.80	173.0
86.80	437.0
87.90	509.0
91.90	274.0
92.80	530.0
94.00	1370.0
94.90	11330.0
96.00	656.0
116.90	115.0
127.80	156.0
142.80	182.0
144.70	116.0
171.70	182.0
173.90	9768.0
174.90	747.0
175.90	9449.0
176.80	624.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
35.80	122.0
37.00	541.0
37.90	508.0
39.00	182.0
39.90	436.0
43.90	334.0
44.80	102.0
46.90	139.0
48.90	455.0
50.00	1962.0
50.90	701.0
56.00	297.0
56.80	307.0
59.90	159.0
61.00	437.0
61.90	473.0
62.80	477.0
64.90	146.0
67.90	943.0
68.90	1155.0
69.90	118.0
73.00	441.0
73.90	2025.0
75.00	5100.0
75.90	480.0
78.80	308.0
79.70	117.0
80.90	358.0
81.80	154.0
86.90	484.0
87.90	451.0
92.00	282.0
92.90	511.0
94.00	1365.0
94.90	10864.0
95.90	665.0
116.90	129.0
118.60	105.0
127.80	140.0
142.80	189.0
144.80	139.0
171.70	198.0
173.90	9813.0
174.90	783.0
175.90	9318.0
176.90	612.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

Scan 2796 (10.080 min): VV012246.D
BFB48

m/z	Abundance
39.90	527.0
43.90	386.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48