




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027388.D
 Acq On : 15 Aug 2022 14:31
 Operator : SY/MD
 Sample : N4096-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBJM7

Manual IntegrationsAPPROVED

Quant Time: Aug 16 03:25:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 16 00:24:20 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/17/2022
 Supervised By :Mahesh Dadoda 08/17/2022

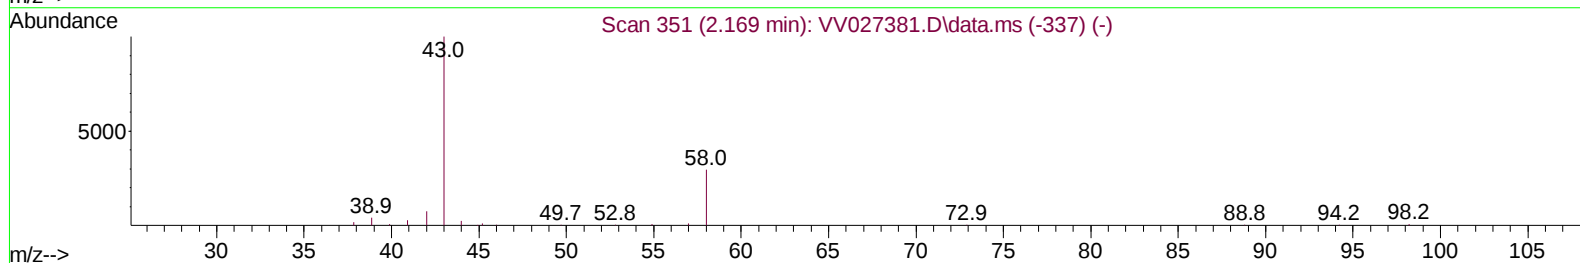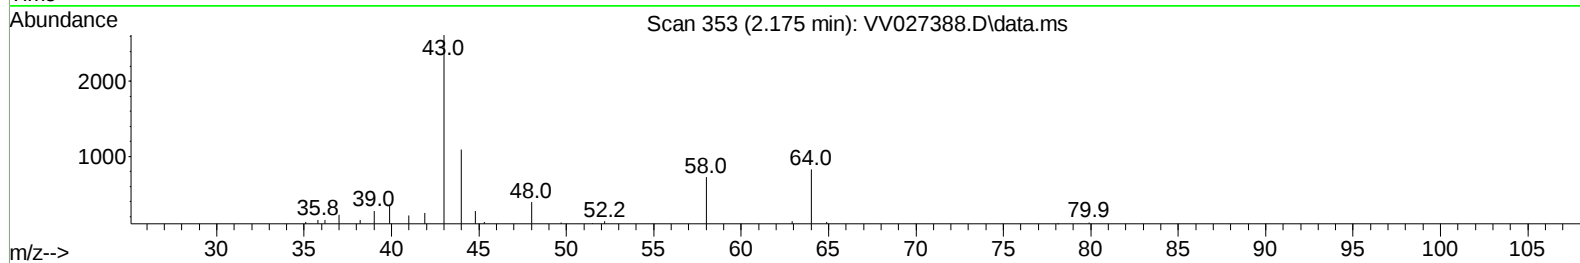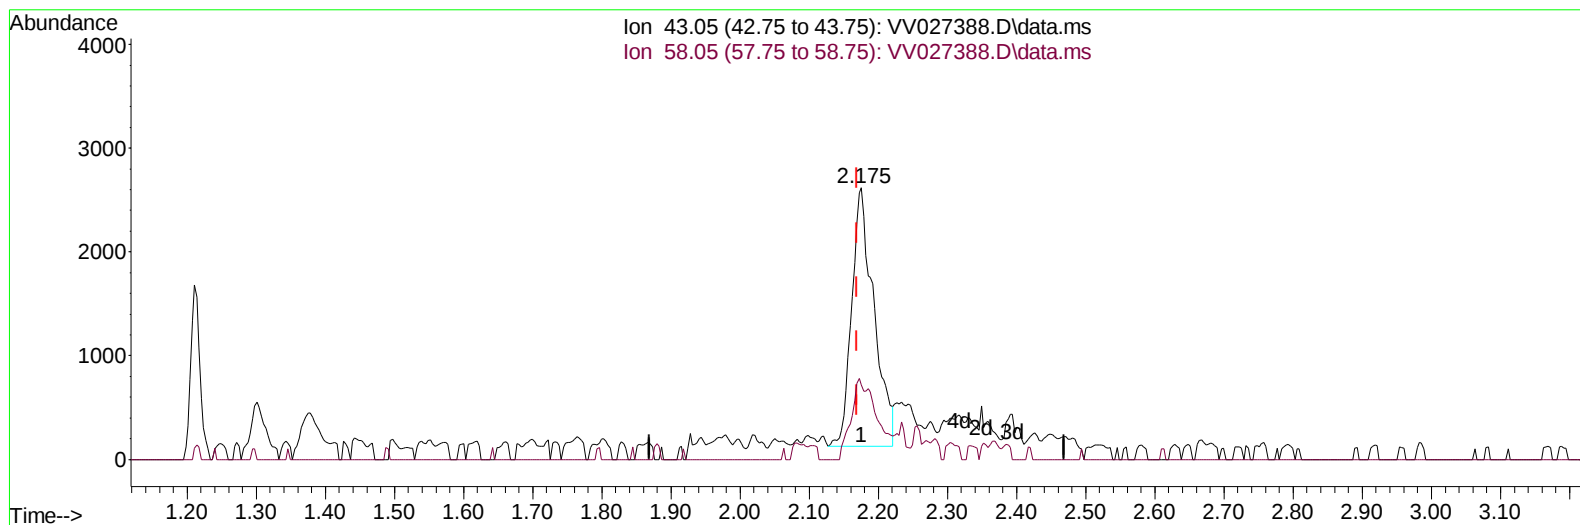

TIC: VV027388.D\data.ms

(13) Acetone (T)

2.175min (+ 0.007) 3.51 ug/L

response 5547

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	31.60	36.13
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027388.D
 Acq On : 15 Aug 2022 14:31
 Operator : SY/MD
 Sample : N4096-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBJM7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/17/2022
 Supervised By :Mahesh Dadoda 08/17/2022

Quant Time: Aug 16 03:25:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 16 00:24:20 2022
 Response via : Initial Calibration

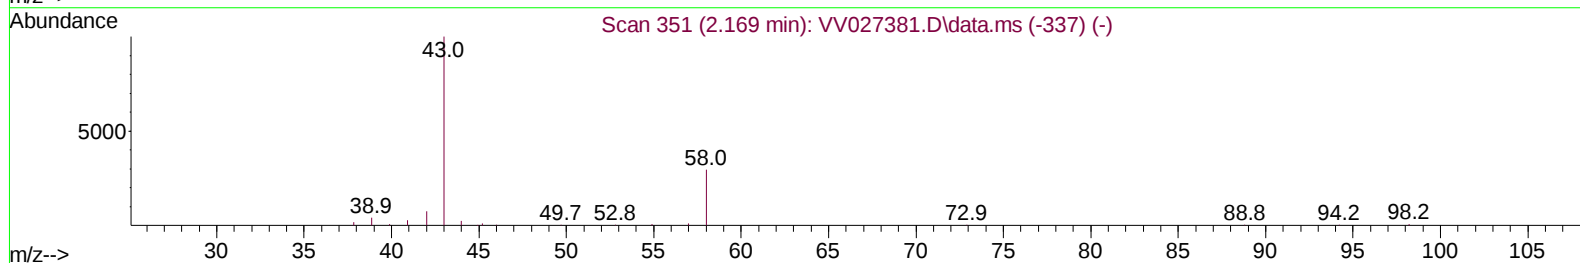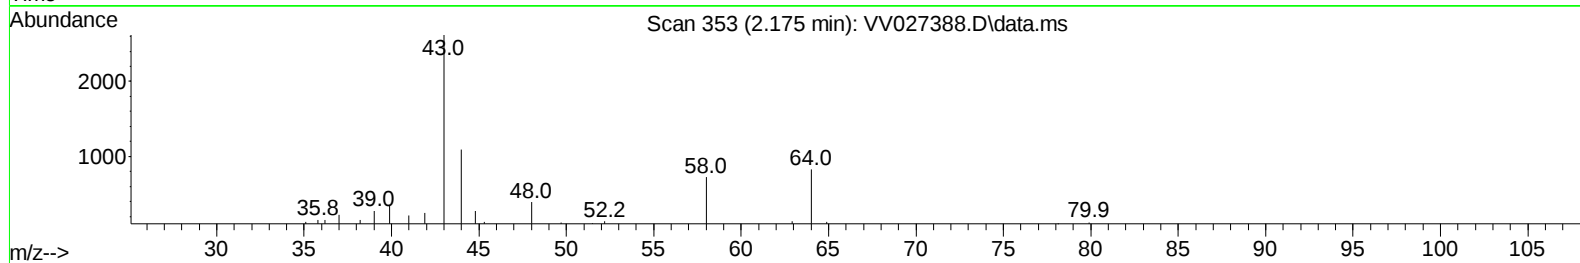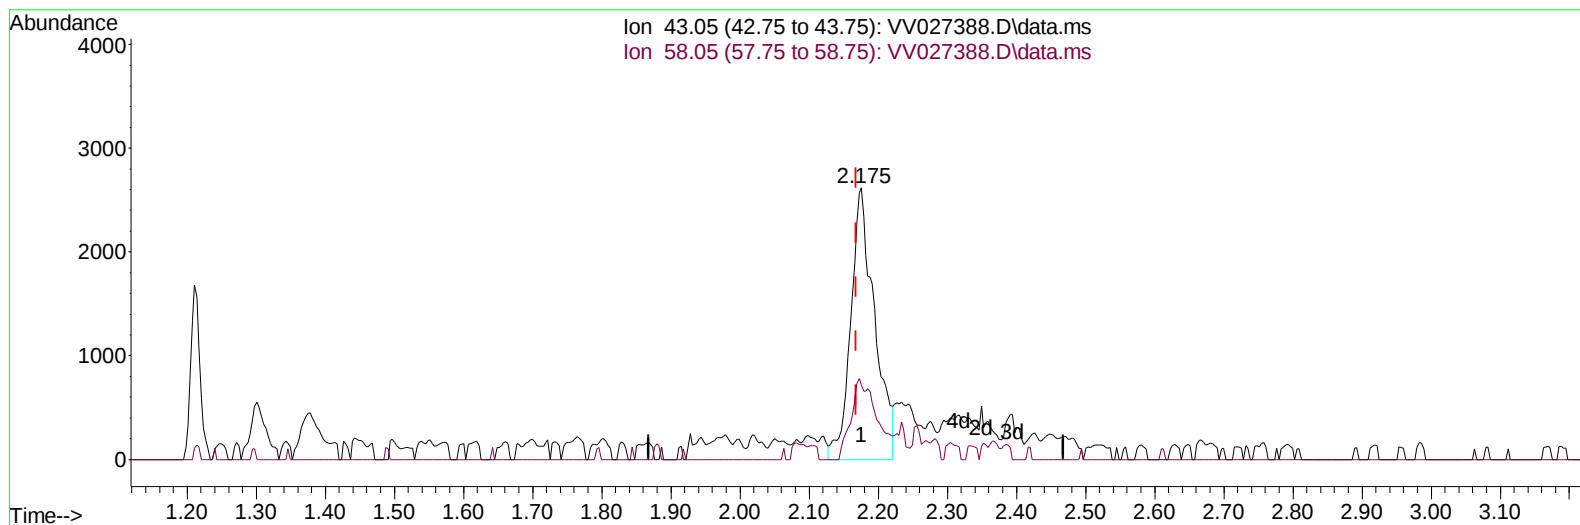

TIC: VV027388.D\data.ms

(13) Acetone (T)

2.175min (+ 0.007) 3.95 ug/L m

response 6247

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	31.60	32.08
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027388.D
 Acq On : 15 Aug 2022 14:31
 Operator : SY/MD
 Sample : N4096-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBJM7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/17/2022
 Supervised By :Mahesh Dadoda 08/17/2022

Quant Time: Aug 16 03:25:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 16 00:24:20 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.616	114		145513	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		157956	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		67674	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.301	65		53262	4.213	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.200%	
7) Chloroethane-d5	1.561	69		40810	4.445	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.800%	
11) 1,1-Dichloroethene-d2	2.102	63		71848	3.134	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.600%	
20) 2-Butanone-d5	3.889	46		111027	51.857	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.720%	
24) Chloroform-d	4.343	84		117022	5.047	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.000%	
26) 1,2-Dichloroethane-d4	5.027	65		56580	5.122	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.400%	
32) Benzene-d6	5.047	84		207127	4.445	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%	
36) 1,2-Dichloropropane-d6	6.066	67		68409	4.748	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.000%	
41) Toluene-d8	7.314	98		169582	3.975	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.600%	
43) trans-1,3-Dichloroprop...	7.622	79		22277	4.464	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.200%	
46) 2-Hexanone-d5	8.088	63		90477	46.848	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.700%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		50761	4.870	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152		60817	5.207	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.200%	
Target Compounds							
13) Acetone	2.175	43		6247m	3.948	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027388.D
Acq On : 15 Aug 2022 14:31
Operator : SY/MD
Sample : N4096-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
GBJM7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/17/2022
Supervised By :Mahesh Dadoda 08/17/2022

Quant Time: Aug 16 03:25:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 16 00:24:20 2022
Response via : Initial Calibration

