




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027395.D
 Acq On : 15 Aug 2022 18:27
 Operator : SY/MD
 Sample : N4195-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CY9

Manual IntegrationsAPPROVED

Quant Time: Aug 16 02:38:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 16 00:24:20 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/17/2022
 Supervised By :Mahesh Dadoda 08/17/2022

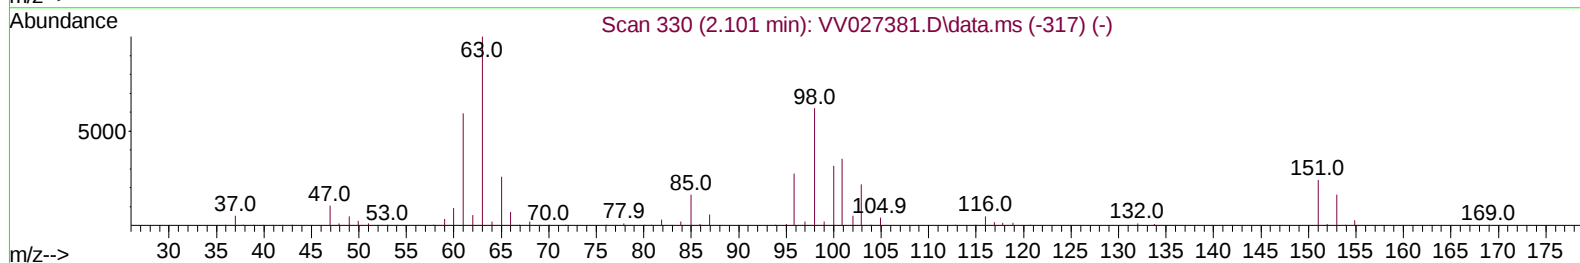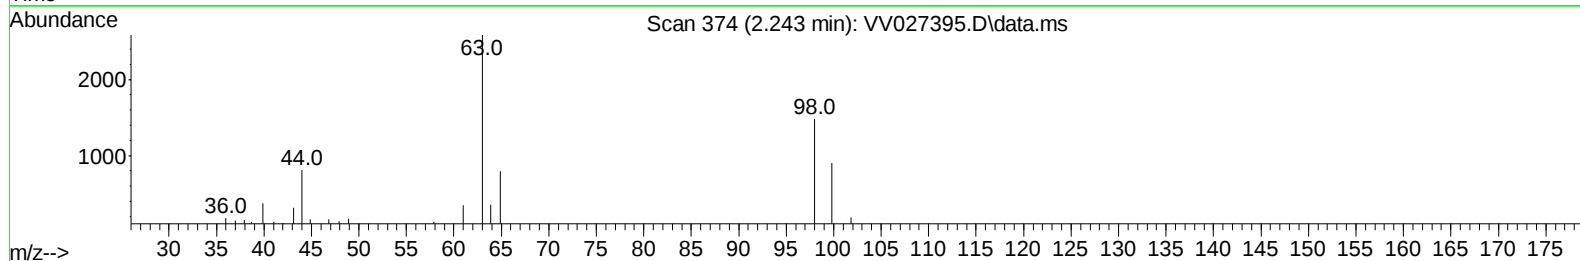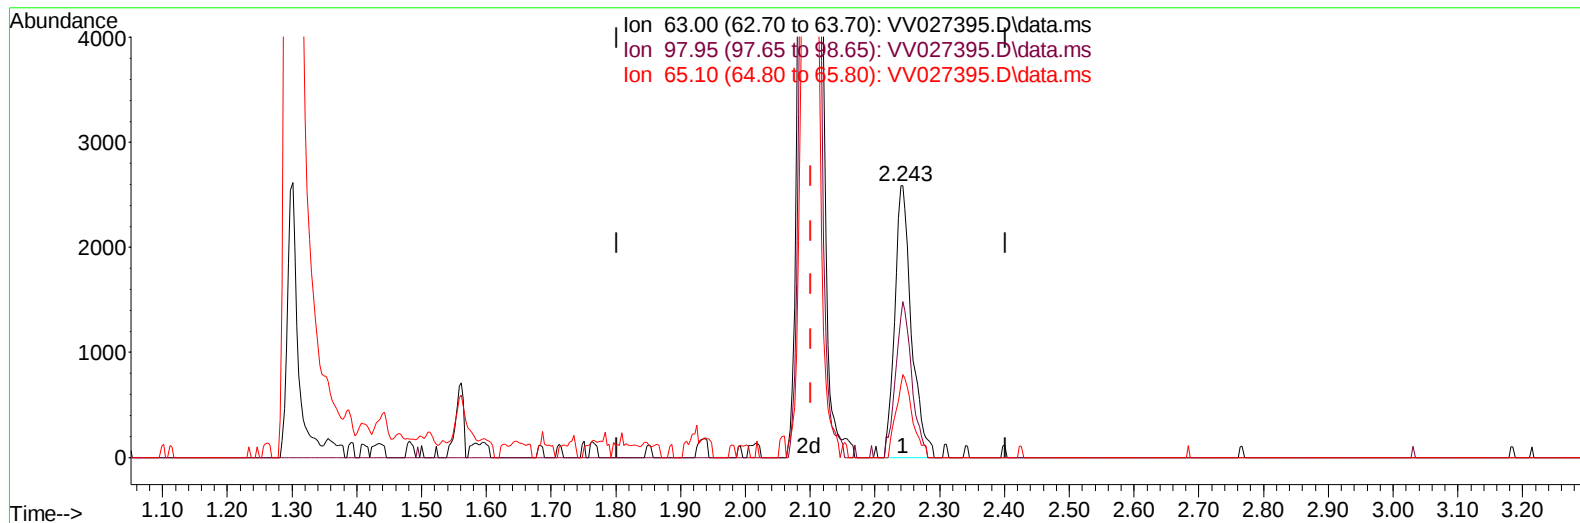

TIC: VV027395.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.243min (+ 0.142) 0.19 ug/L

response 4608

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	55.53
65.10	23.50	29.75
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027395.D
 Acq On : 15 Aug 2022 18:27
 Operator : SY/MD
 Sample : N4195-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CY9

Manual IntegrationsAPPROVED

Quant Time: Aug 16 02:38:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 16 00:24:20 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/17/2022
 Supervised By :Mahesh Dadoda 08/17/2022

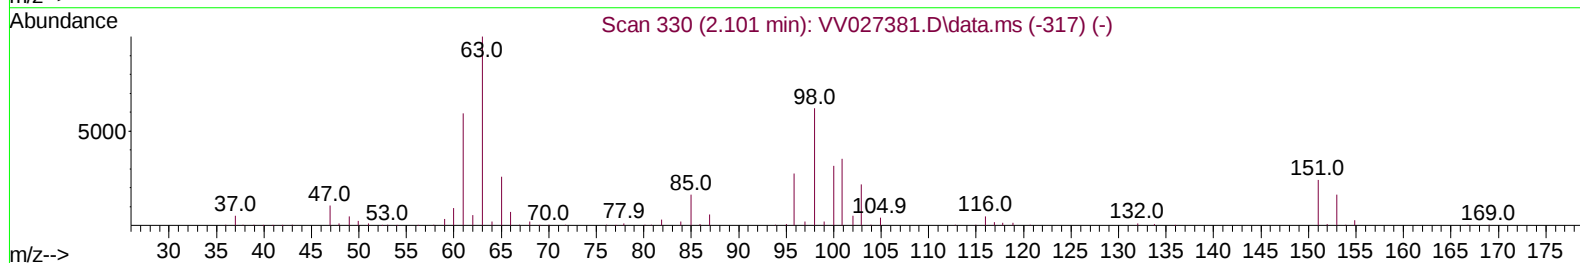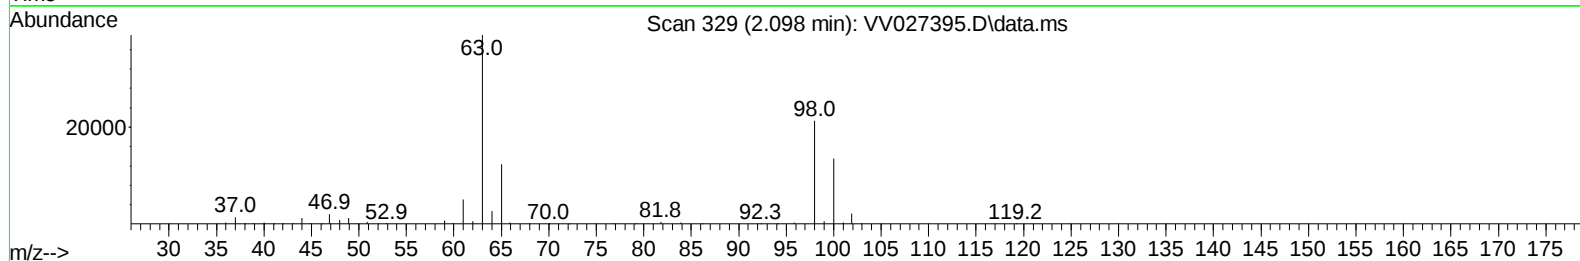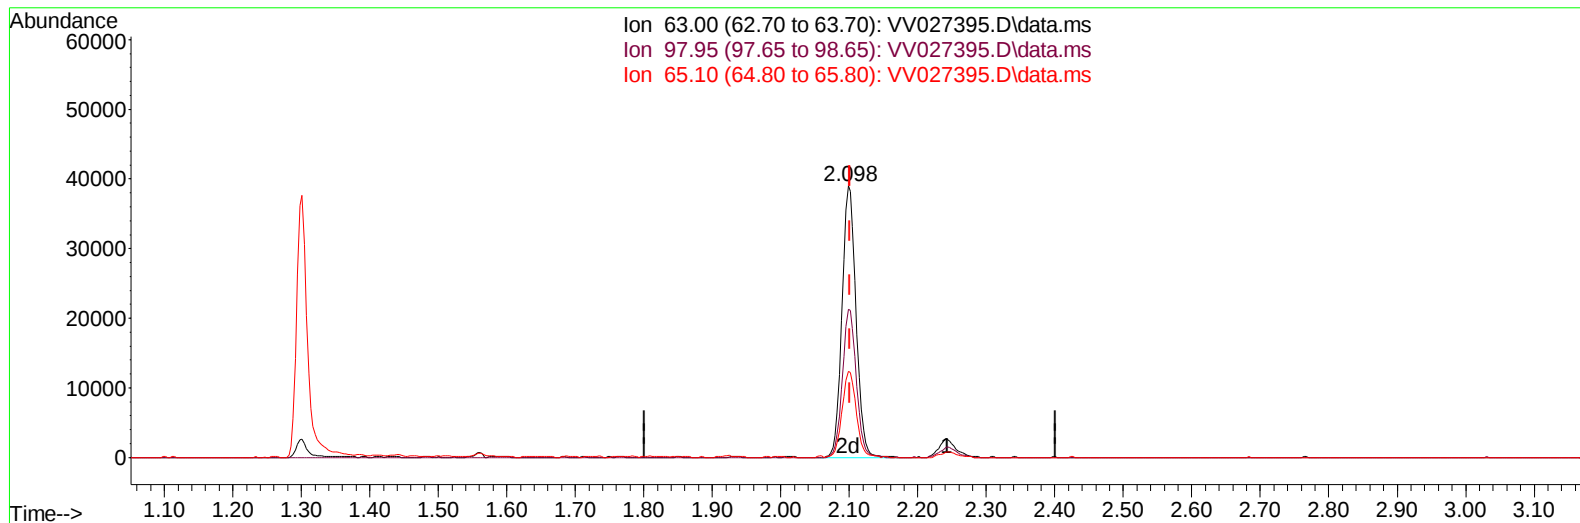

TIC: VV027395.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.098min (-0.003) 2.25 ug/L m

response 55786

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	4.59#
65.10	23.50	2.46#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027395.D
 Acq On : 15 Aug 2022 18:27
 Operator : SY/MD
 Sample : N4195-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CY9

Manual IntegrationsAPPROVED

Quant Time: Aug 16 02:38:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 16 00:24:20 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/17/2022
 Supervised By :Mahesh Dadoda 08/17/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.613	114		157265	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		163073	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		70438	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.301	65		41920	3.068	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	61.400%	
7) Chloroethane-d5	1.561	69		34625	3.489	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	69.800%	
11) 1,1-Dichloroethene-d2	2.098	63		55786m	2.251	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	45.000%#	
20) 2-Butanone-d5	3.886	46		118407	51.171	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.340%	
24) Chloroform-d	4.343	84		96730	3.860	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.200%	
26) 1,2-Dichloroethane-d4	5.031	65		49853	4.176	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.600%	
32) Benzene-d6	5.044	84		178142	3.703	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.000%	
36) 1,2-Dichloropropane-d6	6.066	67		61026	4.103	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.000%	
41) Toluene-d8	7.314	98		140467	3.190	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	63.800%#	
43) trans-1,3-Dichloroprop...	7.622	79		19594	3.803	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.000%	
46) 2-Hexanone-d5	8.088	63		80103	40.175	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.360%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		44637	4.148	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152		55238	4.544	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.800%	
Target Compounds							
34) Trichloroethene	5.915	95		21875	1.577	ug/L	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027395.D
Acq On : 15 Aug 2022 18:27
Operator : SY/MD
Sample : N4195-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
C0CY9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/17/2022
Supervised By :Mahesh Dadoda 08/17/2022

Quant Time: Aug 16 02:38:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 16 00:24:20 2022
Response via : Initial Calibration

