

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027388.D
 Acq On : 15 Aug 2022 14:31
 Operator : SY/MD
 Sample : N4096-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBJM7

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 08/17/2022
 Supervised By :Mahesh Dadoda 08/17/2022

Quant Time: Aug 16 03:25:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 16 00:24:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	145513	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	157956	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	67674	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	53262	4.213	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	84.200%	
7) Chloroethane-d5	1.561	69	40810	4.445	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	88.800%	
11) 1,1-Dichloroethene-d2	2.102	63	71848	3.134	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	62.600%	
20) 2-Butanone-d5	3.889	46	111027	51.857	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	103.720%	
24) Chloroform-d	4.343	84	117022	5.047	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.000%	
26) 1,2-Dichloroethane-d4	5.027	65	56580	5.122	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.400%	
32) Benzene-d6	5.047	84	207127	4.445	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	89.000%	
36) 1,2-Dichloropropane-d6	6.066	67	68409	4.748	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	95.000%	
41) Toluene-d8	7.314	98	169582	3.975	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	79.600%	
43) trans-1,3-Dichloroprop...	7.622	79	22277	4.464	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	89.200%	
46) 2-Hexanone-d5	8.088	63	90477	46.848	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	93.700%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	50761	4.870	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	97.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	60817	5.207	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	104.200%	
Target Compounds					Qvalue	
13) Acetone	2.175	43	6247m	3.948	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027388.D
Acq On : 15 Aug 2022 14:31
Operator : SY/MD
Sample : N4096-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
GBJM7

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 08/17/2022
Supervised By :Mahesh Dadoda 08/17/2022

Quant Time: Aug 16 03:25:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 16 00:24:20 2022
Response via : Initial Calibration

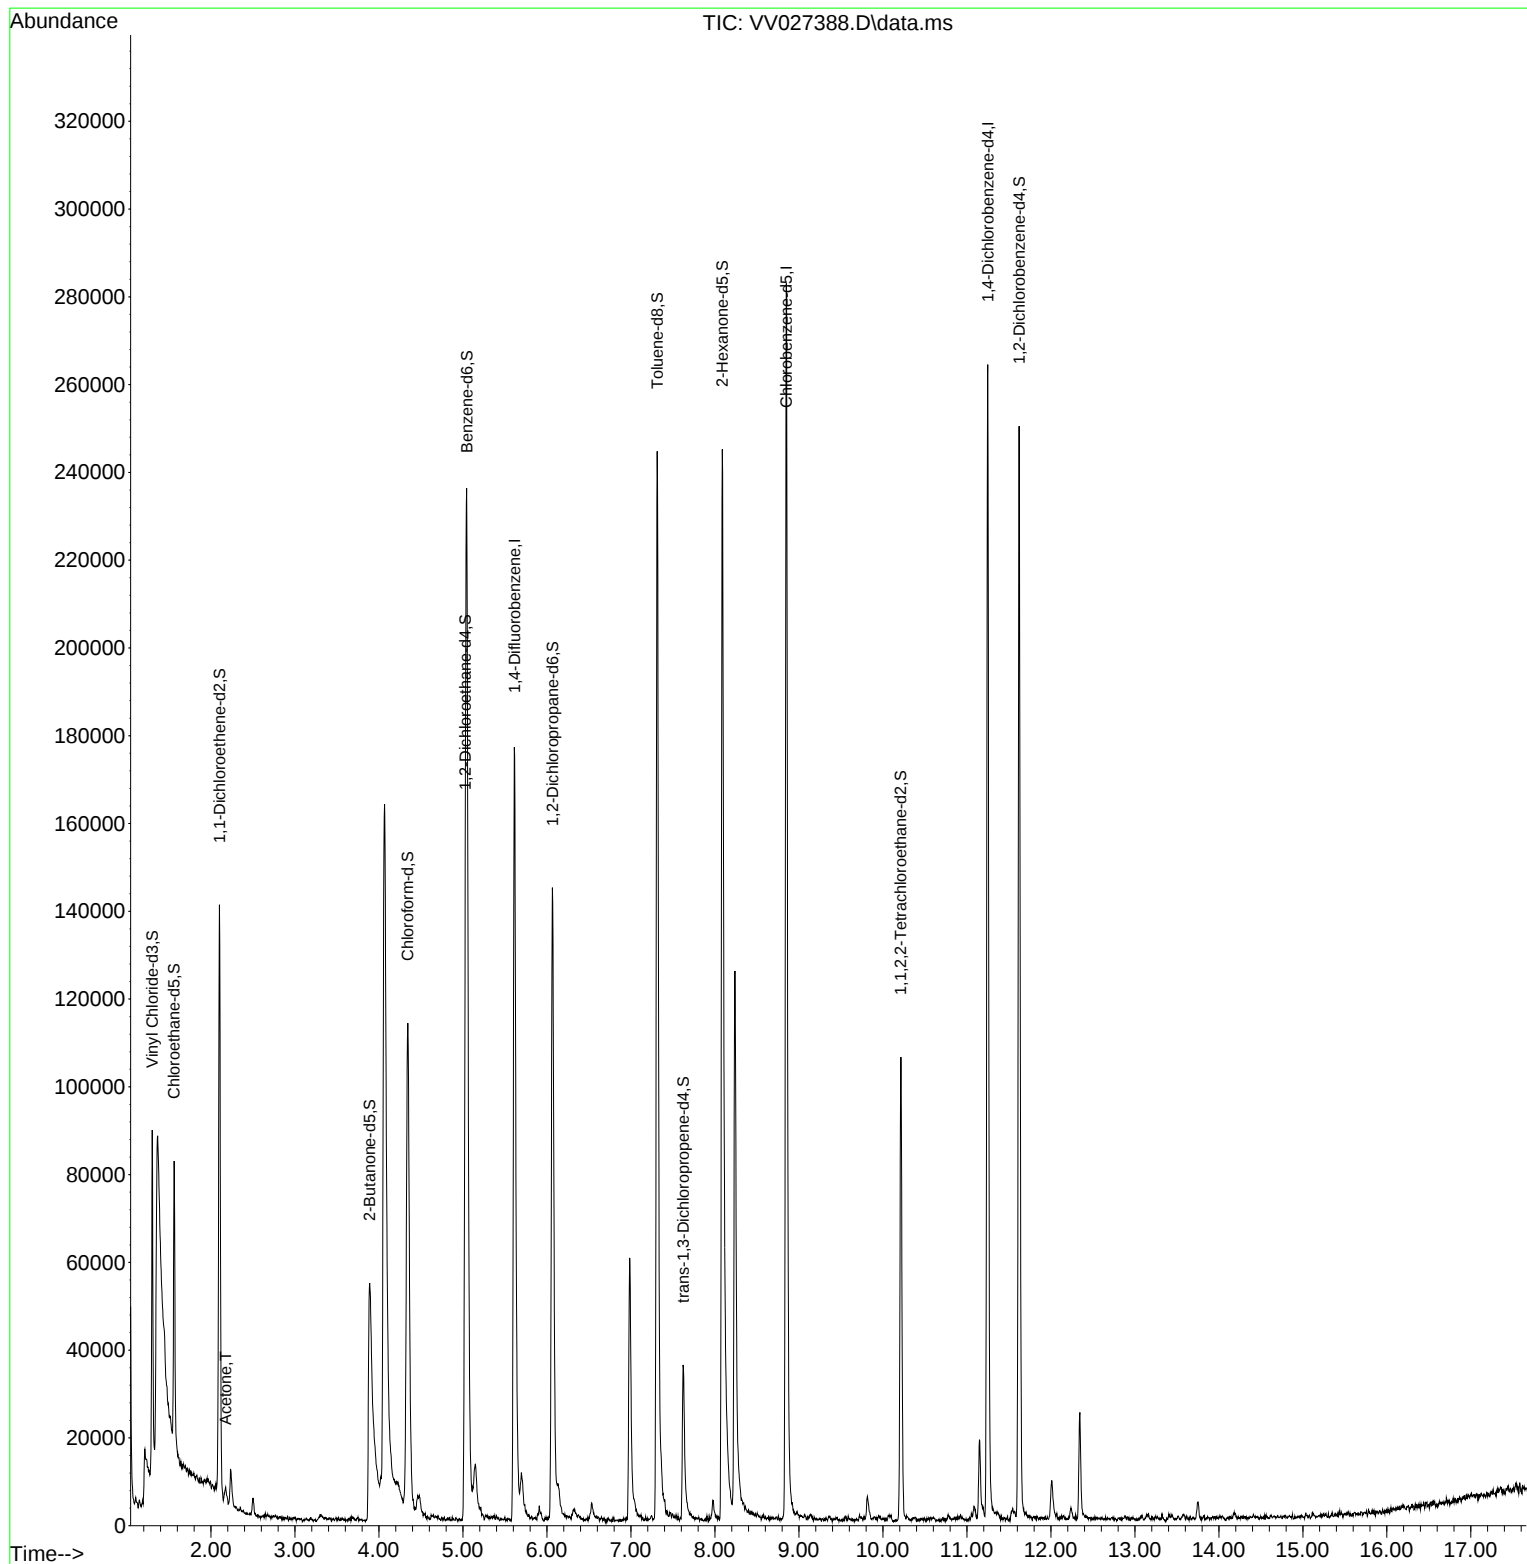

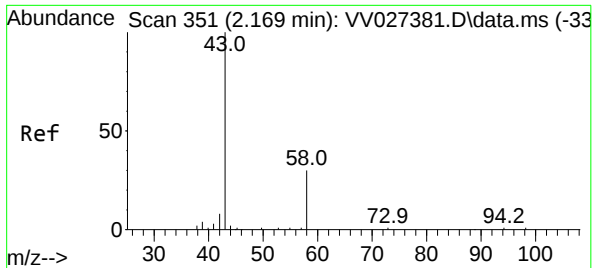

#13

Acetone

Concen: 3.948 ug/L m

RT: 2.175 min Scan# 3

Delta R.T. 0.007 min

Lab File: VV027388.D

Acq: 15 Aug 2022 14:31

Instrument :

MSVOA_V

ClientSampleId :

GBJM7

Tgt Ion: 43 Resp: 624

Ion Ratio Lower Upper

43 100

58 32.1 0.0 63.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 08/17/2022

Supervised By :Mahesh Dadoda 08/17/2022

