

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW081522\
 Data File : VW027389.D
 Acq On : 15 Aug 2022 14:56
 Operator : SY/MD
 Sample : N4096-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBJM9

Quant Time: Aug 16 02:37:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 16 00:24:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	146873	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	159537	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	65738	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	49296	3.863	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.200%
7) Chloroethane-d5	1.561	69	40312	4.350	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.000%
11) 1,1-Dichloroethene-d2	2.101	63	69212	2.991	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.800%#
20) 2-Butanone-d5	3.892	46	113648	52.589	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.180%
24) Chloroform-d	4.342	84	113993	4.871	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.400%
26) 1,2-Dichloroethane-d4	5.030	65	56004	5.023	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.400%
32) Benzene-d6	5.043	84	202997	4.313	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.200%
36) 1,2-Dichloropropane-d6	6.066	67	66702	4.584	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.600%
41) Toluene-d8	7.313	98	163971	3.806	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.200%
43) trans-1,3-Dichloroprop...	7.622	79	21703	4.306	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.200%
46) 2-Hexanone-d5	8.088	63	87941	45.084	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.160%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	48099	4.569	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	59445	5.239	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.800%
Target Compounds						
					Qvalue	
13) Acetone	2.175	43	6229	3.901	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027389.D
Acq On : 15 Aug 2022 14:56
Operator : SY/MD
Sample : N4096-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBJM9

Quant Time: Aug 16 02:37:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 16 00:24:20 2022
Response via : Initial Calibration

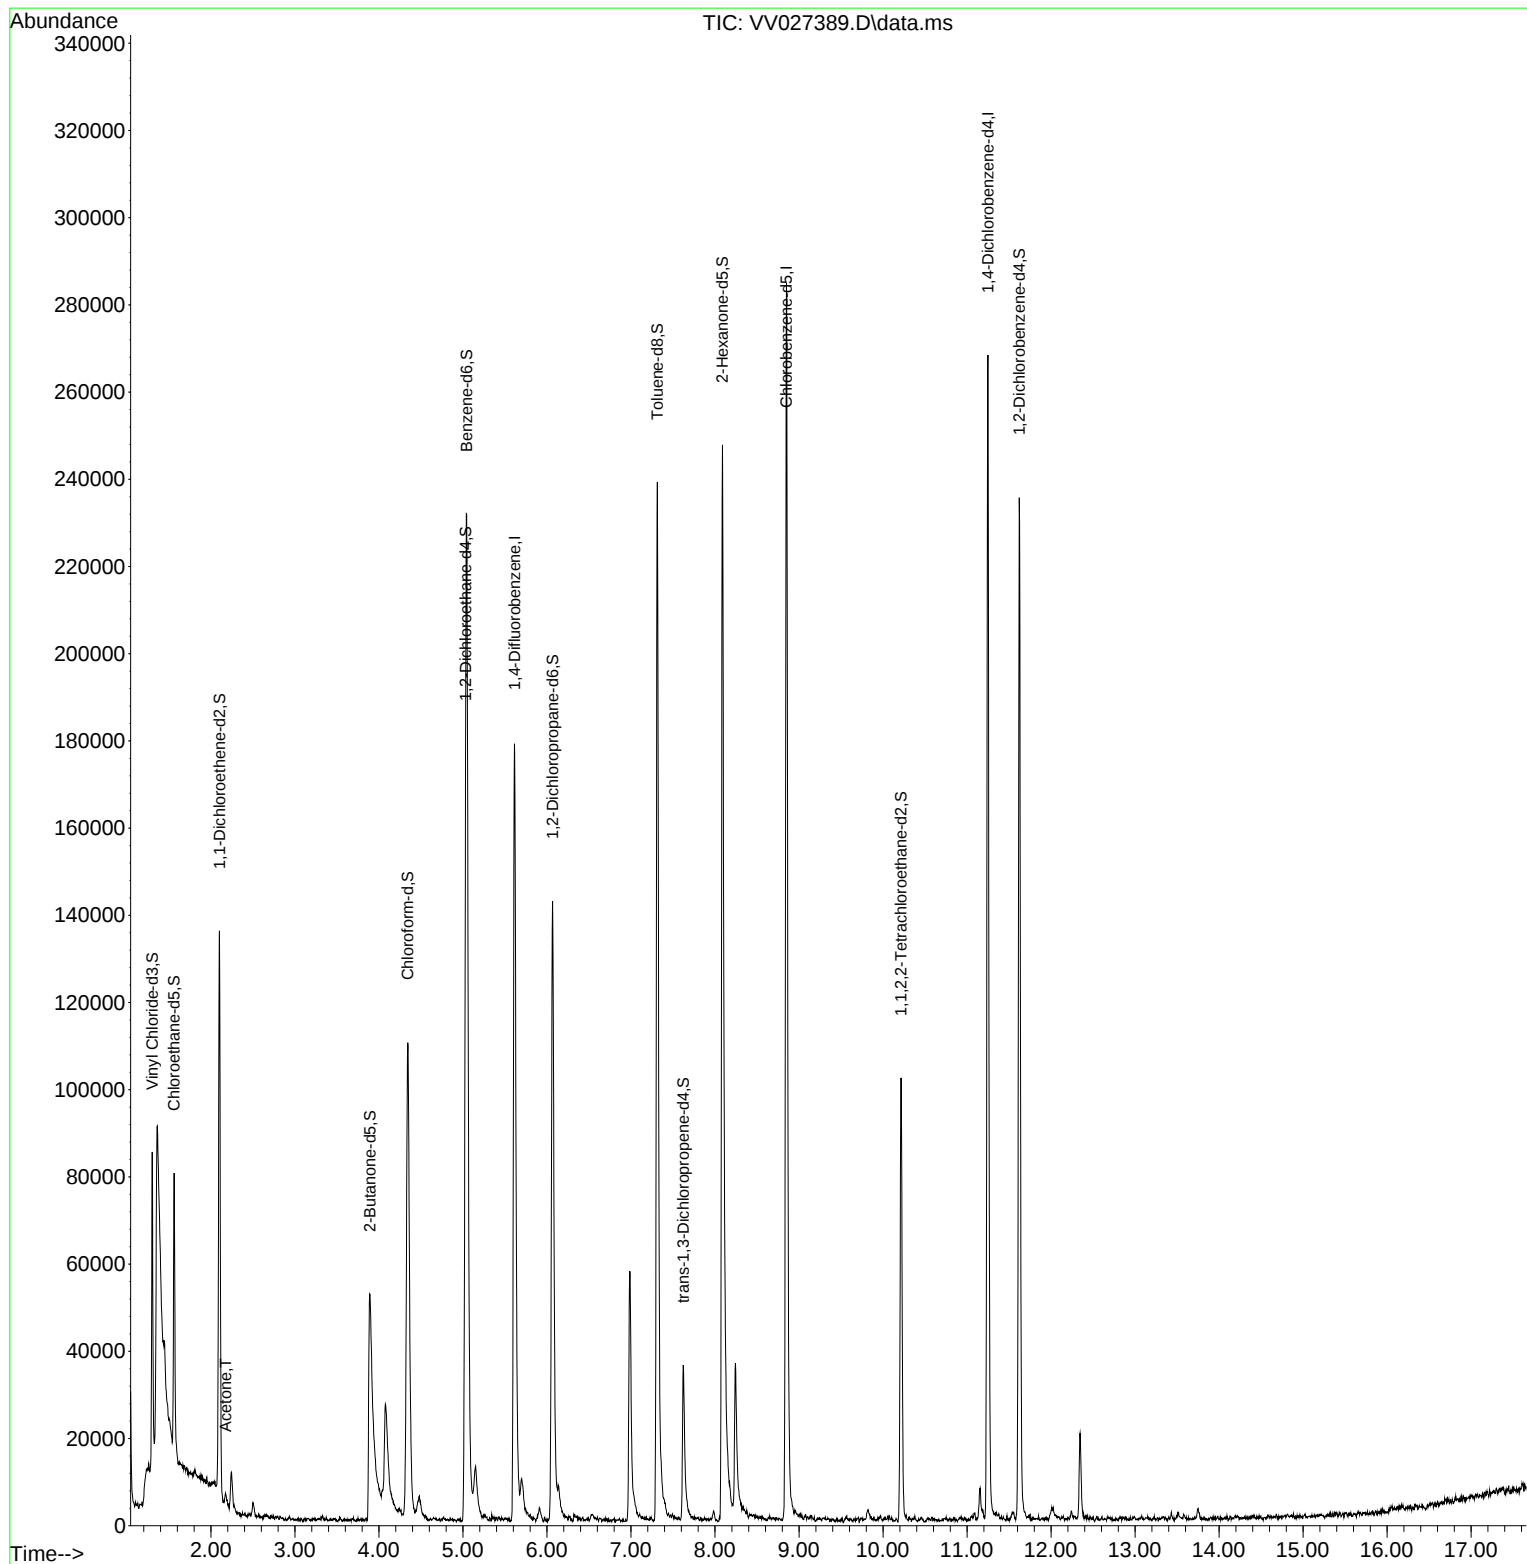

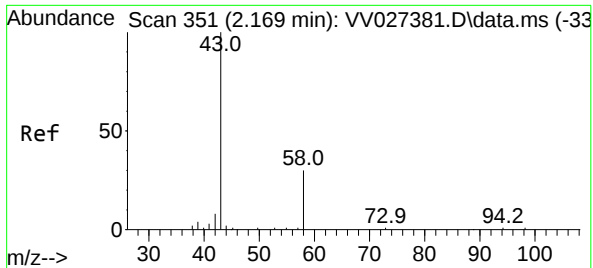

#13

Acetone

Concen: 3.901 ug/L

RT: 2.175 min Scan# 3

Delta R.T. 0.006 min

Lab File: VV027389.D


Acq: 15 Aug 2022 14:56

Instrument :

MSVOA_V

ClientSampleId :

GBJM9

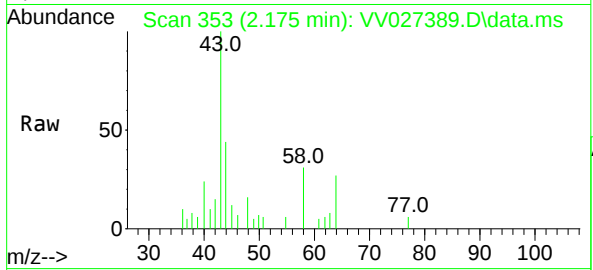

Tgt Ion: 43 Resp: 6229

Ion Ratio Lower Upper

43 100

58 27.0 0.0 63.2

