

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027392.D
 Acq On : 15 Aug 2022 16:47
 Operator : SY/MD
 Sample : N4192-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB6

Quant Time: Aug 16 02:38:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 16 00:24:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	177270	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	183865	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	79600	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	49607	3.221	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	64.400%
7) Chloroethane-d5	1.561	69	40186	3.593	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	71.800%
11) 1,1-Dichloroethene-d2	2.101	63	63366	2.269	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	45.400%#
20) 2-Butanone-d5	3.873	46	126300	48.422	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.840%
24) Chloroform-d	4.342	84	109505	3.877	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.600%
26) 1,2-Dichloroethane-d4	5.027	65	54108	4.021	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.400%
32) Benzene-d6	5.047	84	196790	3.628	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	72.600%
36) 1,2-Dichloropropane-d6	6.066	67	65699	3.918	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	78.400%
41) Toluene-d8	7.313	98	158663	3.195	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	64.000%#
43) trans-1,3-Dichloroprop...	7.622	79	21561	3.712	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.200%
46) 2-Hexanone-d5	8.085	63	87623	38.977	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.960%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	47981	3.955	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	61012	4.441	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.800%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	7588	0.370	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027392.D
Acq On : 15 Aug 2022 16:47
Operator : SY/MD
Sample : N4192-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB6

Quant Time: Aug 16 02:38:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 16 00:24:20 2022
Response via : Initial Calibration

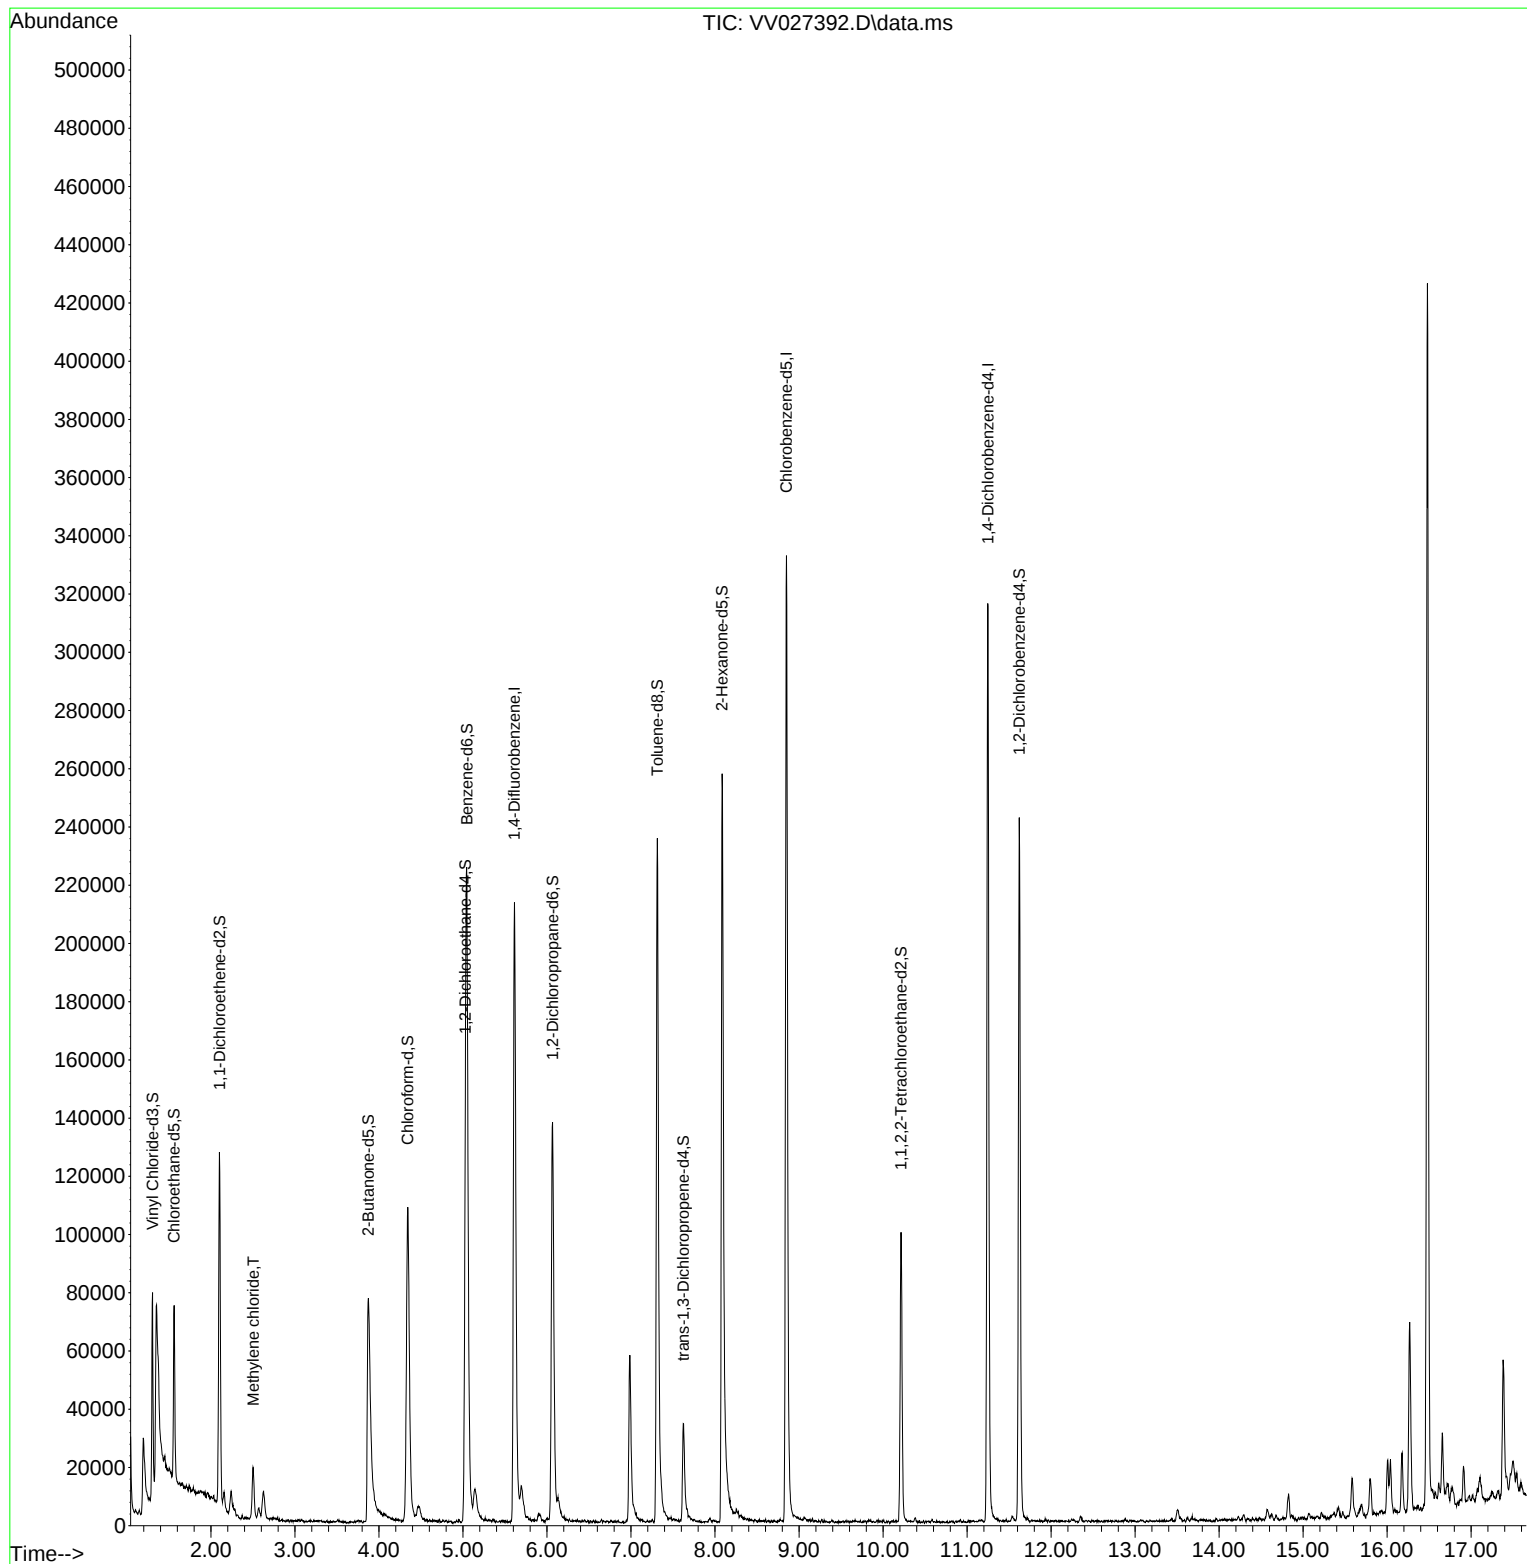

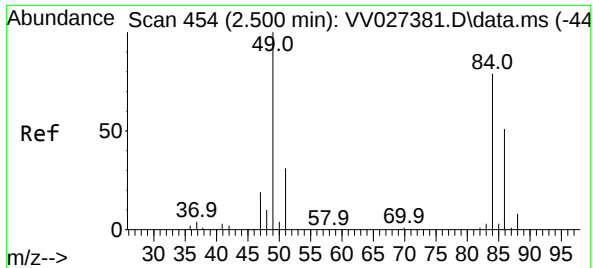

#16
Methylene chloride
Concen: 0.370 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV027392.D
Acq: 15 Aug 2022 16:47

Instrument :
MSVOA_V
ClientSampleId :
C0AB6

Tgt Ion:	84	Resp:	7588
Ion	Ratio	Lower	Upper
84	100		
86	55.4	45.1	83.9
49	117.9	91.2	169.4

