

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027396.D
 Acq On : 15 Aug 2022 18:52
 Operator : SY/MD
 Sample : N4195-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CZ0

Quant Time: Aug 16 02:38:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 16 00:24:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	141491	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	149537	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62283	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	44219	3.597	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.000%
7) Chloroethane-d5	1.561	69	36295	4.065	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.400%
11) 1,1-Dichloroethene-d2	2.101	63	59812	2.683	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	53.600%#
20) 2-Butanone-d5	3.889	46	115221	55.345	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.700%
24) Chloroform-d	4.346	84	105773	4.692	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.800%
26) 1,2-Dichloroethane-d4	5.030	65	54414	5.066	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.400%
32) Benzene-d6	5.047	84	185585	4.207	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.200%
36) 1,2-Dichloropropane-d6	6.066	67	64306	4.715	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.200%
41) Toluene-d8	7.313	98	148074	3.667	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.400%
43) trans-1,3-Dichloroprop...	7.622	79	20788	4.400	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.000%
46) 2-Hexanone-d5	8.088	63	88643	48.483	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.960%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	47230	4.787	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	57614	5.359	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.200%
Target Compounds						
					Qvalue	
13) Acetone	2.175	43	12895	8.382	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027396.D
Acq On : 15 Aug 2022 18:52
Operator : SY/MD
Sample : N4195-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CZ0

Quant Time: Aug 16 02:38:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 16 00:24:20 2022
Response via : Initial Calibration

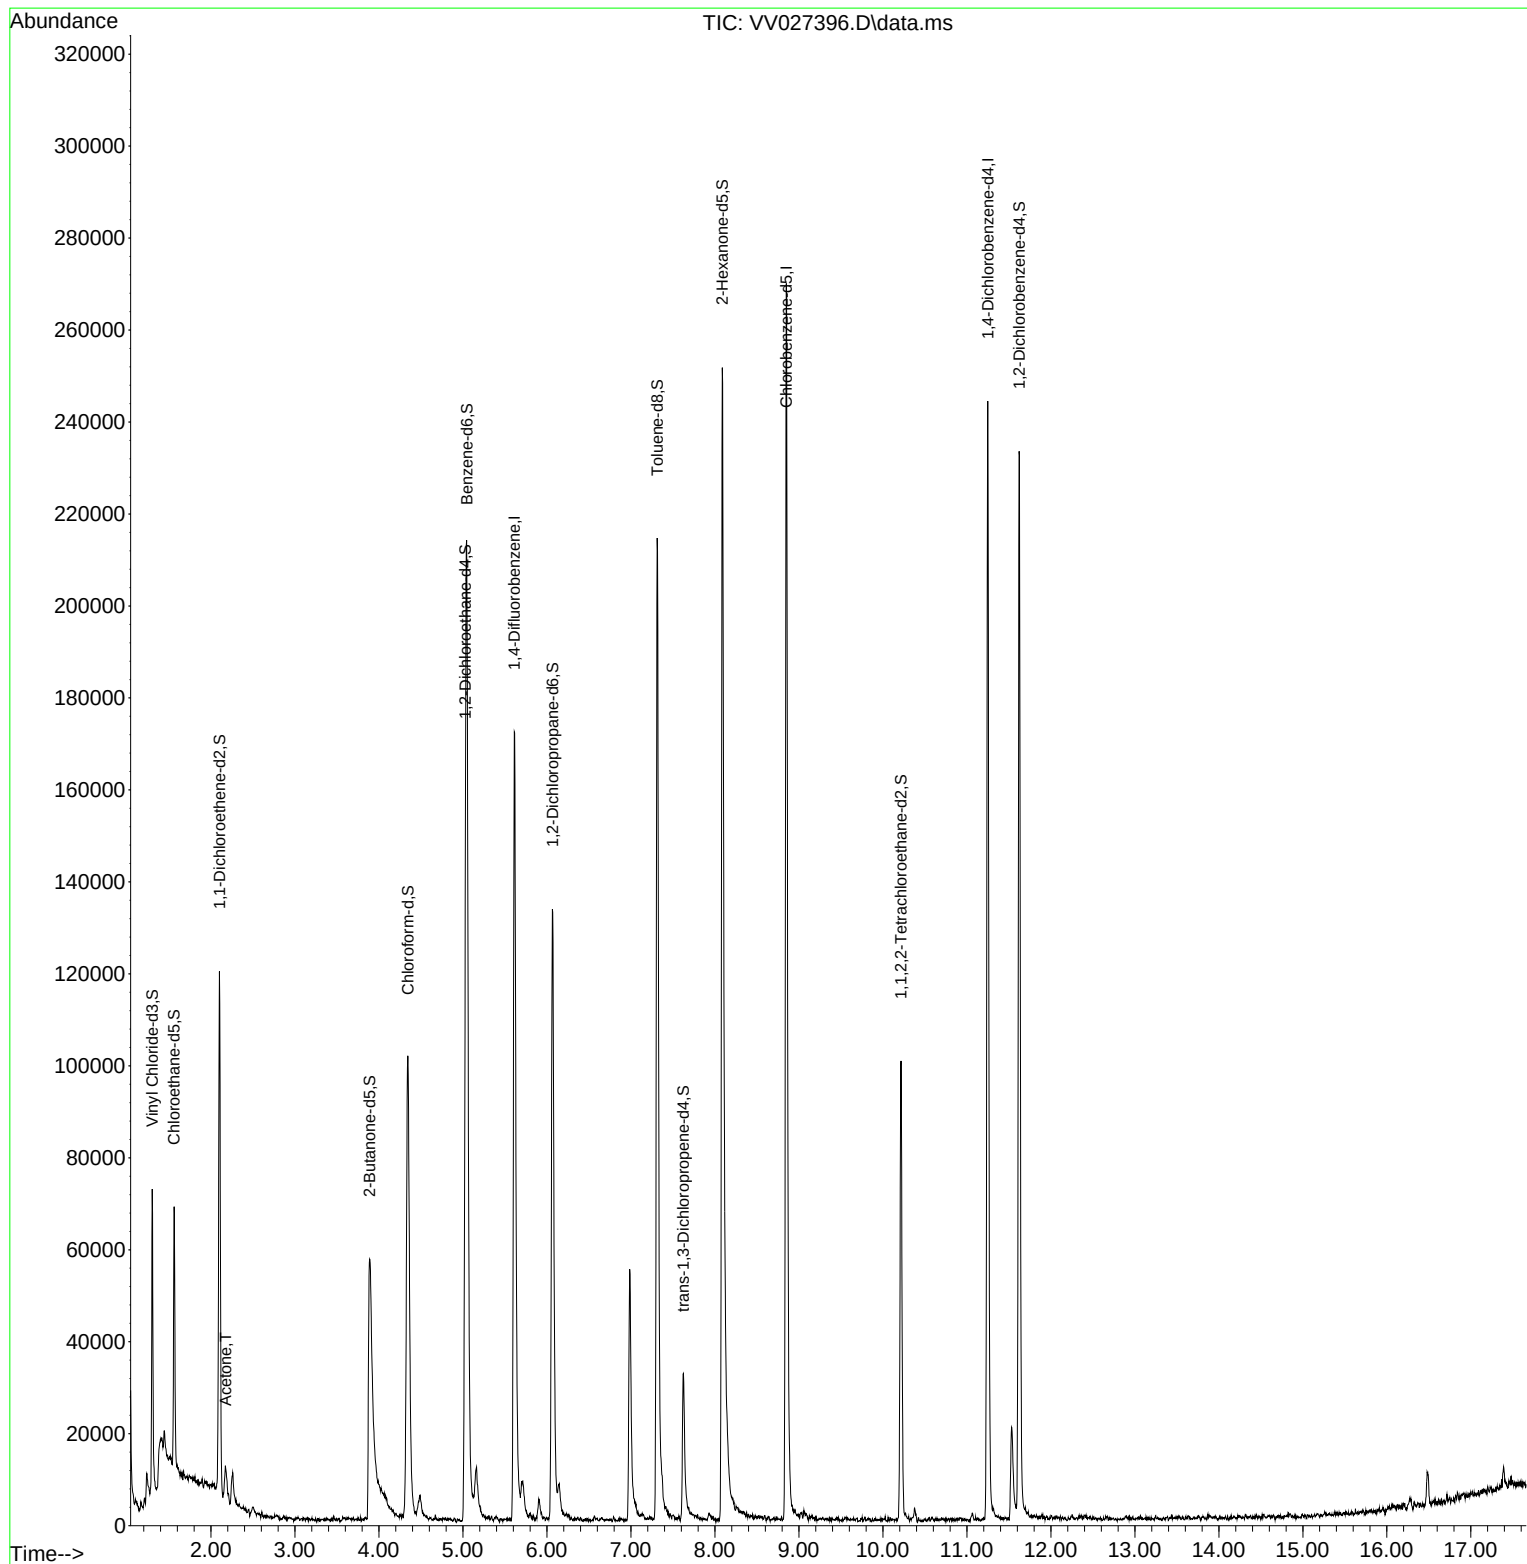

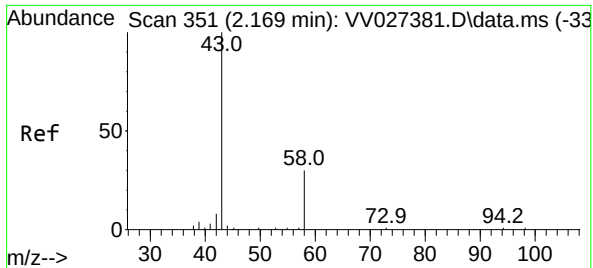

#13
 Acetone
 Concen: 8.382 ug/L
 RT: 2.175 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VV027396.D
 Acq: 15 Aug 2022 18:52

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CZ0

Tgt Ion: 43 Resp: 12895
 Ion Ratio Lower Upper
 43 100
 58 31.4 0.0 63.2

