

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027397.D
 Acq On : 15 Aug 2022 19:17
 Operator : SY/MD
 Sample : N4195-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CZ1

Quant Time: Aug 16 02:39:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 16 00:24:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	141584	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	151575	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61200	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	43697	3.552	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.000%
7) Chloroethane-d5	1.564	69	36368	4.071	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.400%
11) 1,1-Dichloroethene-d2	2.101	63	60468	2.711	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	54.200%#
20) 2-Butanone-d5	3.889	46	101089	48.525	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.060%
24) Chloroform-d	4.342	84	104798	4.645	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.000%
26) 1,2-Dichloroethane-d4	5.030	65	52525	4.887	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.800%
32) Benzene-d6	5.047	84	182434	4.080	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.600%
36) 1,2-Dichloropropane-d6	6.069	67	62609	4.529	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.600%
41) Toluene-d8	7.313	98	147329	3.599	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.000%
43) trans-1,3-Dichloroprop...	7.625	79	20340	4.247	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.000%
46) 2-Hexanone-d5	8.088	63	86286	46.559	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.120%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	46549	4.654	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	57324	5.427	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.600%
Target Compounds					Qvalue	
13) Acetone	2.169	43	9823	6.381	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027397.D
Acq On : 15 Aug 2022 19:17
Operator : SY/MD
Sample : N4195-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CZ1

Quant Time: Aug 16 02:39:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 16 00:24:20 2022
Response via : Initial Calibration

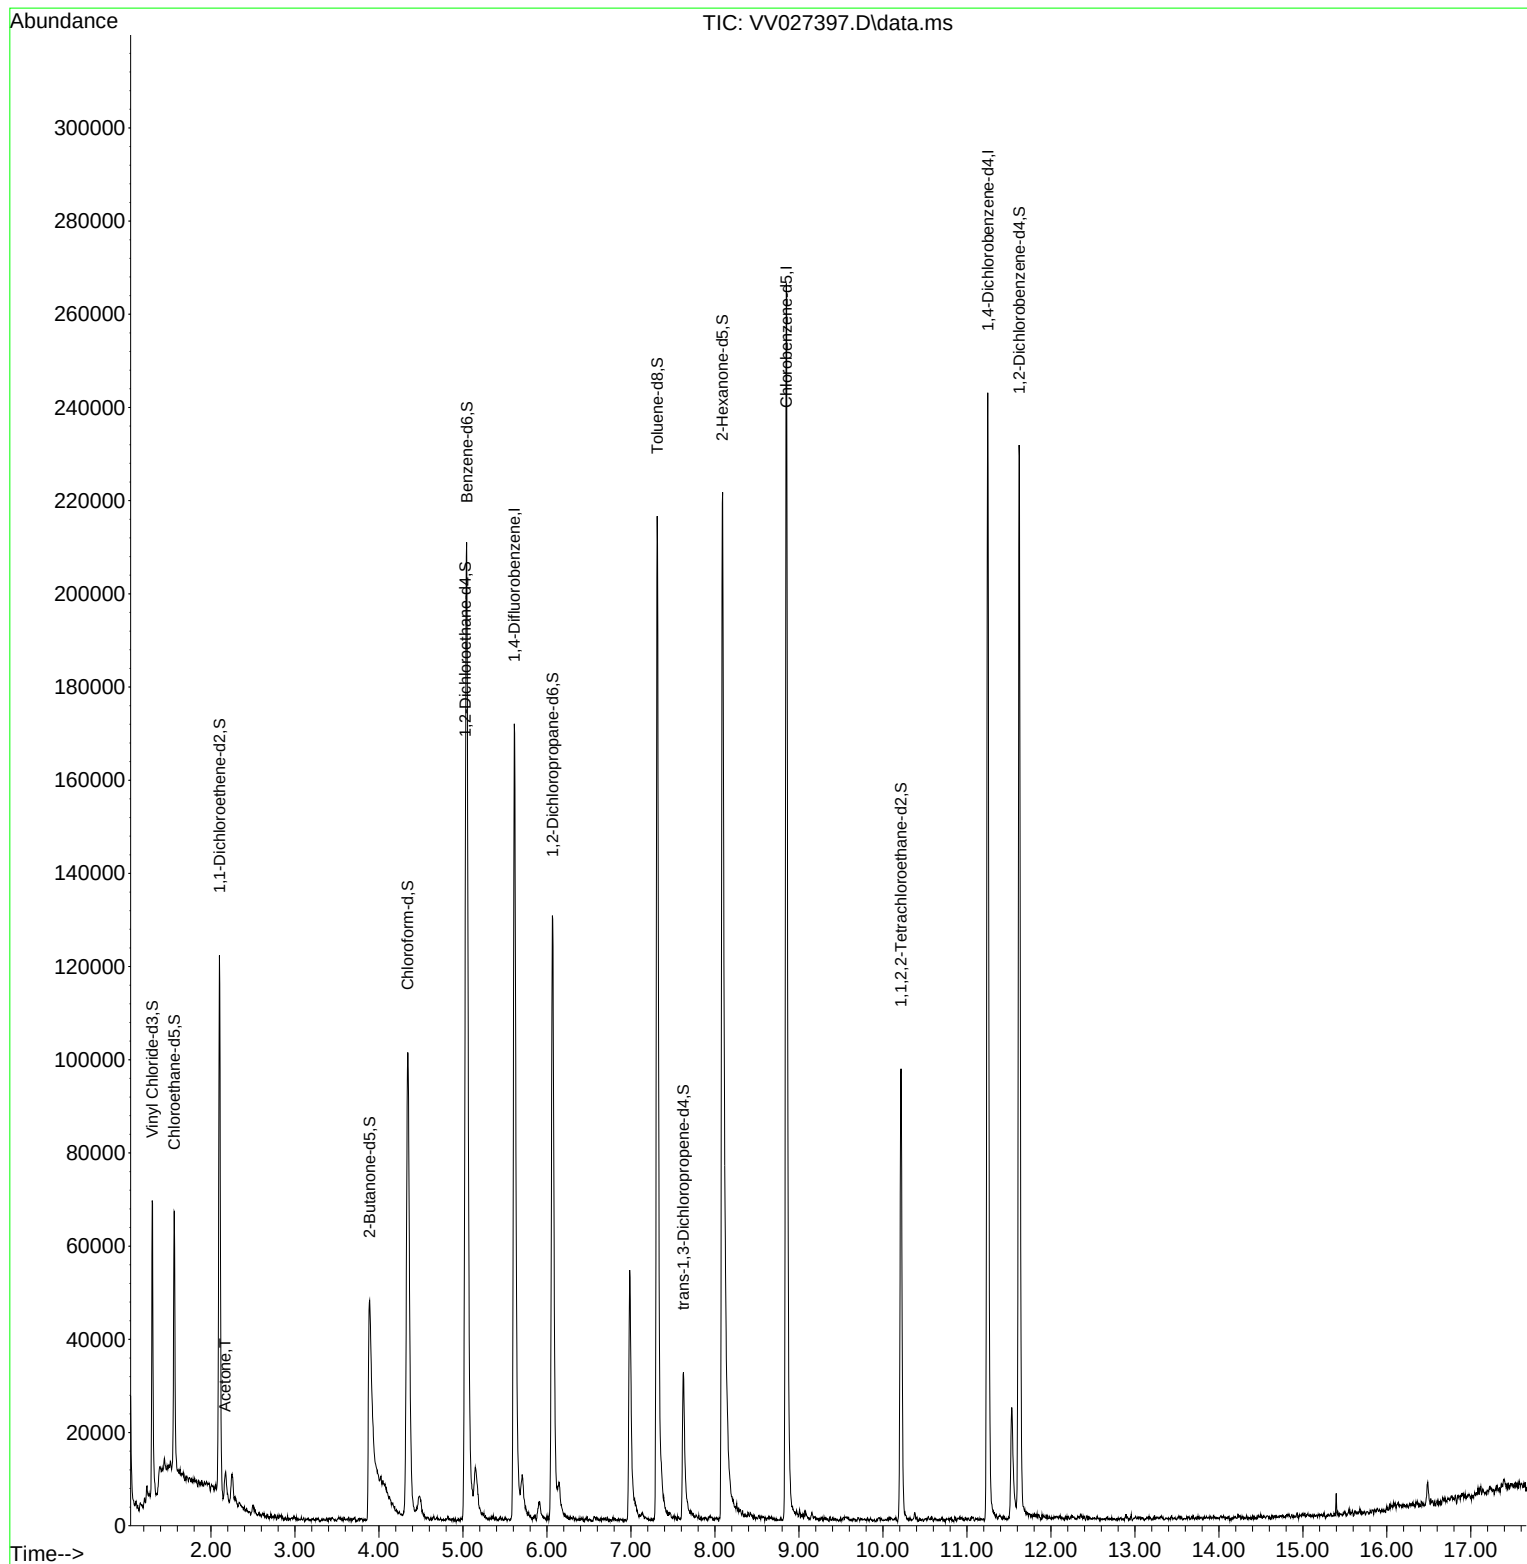

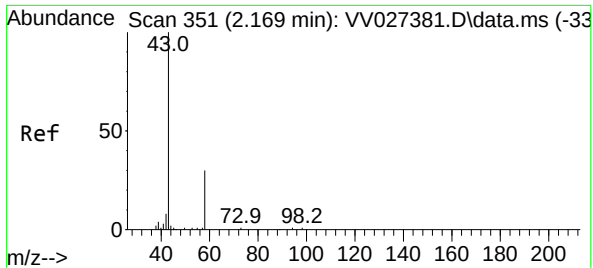

#13
 Acetone
 Concen: 6.381 ug/L
 RT: 2.169 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VV027397.D
 Acq: 15 Aug 2022 19:17

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CZ1

Tgt Ion: 43 Resp: 9823
 Ion Ratio Lower Upper
 43 100
 58 35.6 0.0 63.2

