

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027383.D
 Acq On : 15 Aug 2022 12:30
 Operator : SY/MD
 Sample : N4162-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027383.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	21	27	35	rVB3	10261	13590	2.22%	0.281%
2	1.301	73	81	93	rBV	81113	88058	14.41%	1.820%
3	1.375	96	104	110	rBV2	8520	16386	2.68%	0.339%
4	1.561	155	162	173	rVB	70769	81902	13.40%	1.692%
5	2.101	320	330	342	rVB	147338	214552	35.11%	4.434%
6	2.214	356	365	379	rVB4	8240	17930	2.93%	0.371%
7	2.503	445	455	466	rVB2	13981	25143	4.11%	0.520%
8	3.886	876	885	915	rBV2	43323	149717	24.50%	3.094%
9	4.346	1011	1028	1052	rBV	110663	287808	47.09%	5.947%
10	5.043	1228	1245	1263	rBV3	245414	611137	100.00%	12.629%
11	5.612	1410	1422	1438	rBV	167484	343438	56.20%	7.097%
12	5.911	1505	1515	1530	rBV	4289	9062	1.48%	0.187%
13	6.066	1550	1563	1593	rBV	148923	327302	53.56%	6.763%
14	6.985	1839	1849	1882	rBV	65465	135106	22.11%	2.792%
15	7.313	1940	1951	1980	rBV	262408	489632	80.12%	10.118%
16	7.622	2038	2047	2067	rBV2	35489	71640	11.72%	1.480%
17	8.088	2179	2192	2233	rBV	217236	539430	88.27%	11.147%
18	8.850	2417	2429	2452	rBV	265955	459438	75.18%	9.494%
19	10.217	2840	2854	2873	rBV	102717	170941	27.97%	3.532%
20	11.249	3163	3175	3196	rBV	243440	387185	63.35%	8.001%
21	11.622	3280	3291	3311	rBV	244471	399894	65.43%	8.263%




Sum of corrected areas: 4839291

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027383.D
Acq On : 15 Aug 2022 12:30
Operator : SY/MD
Sample : N4162-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

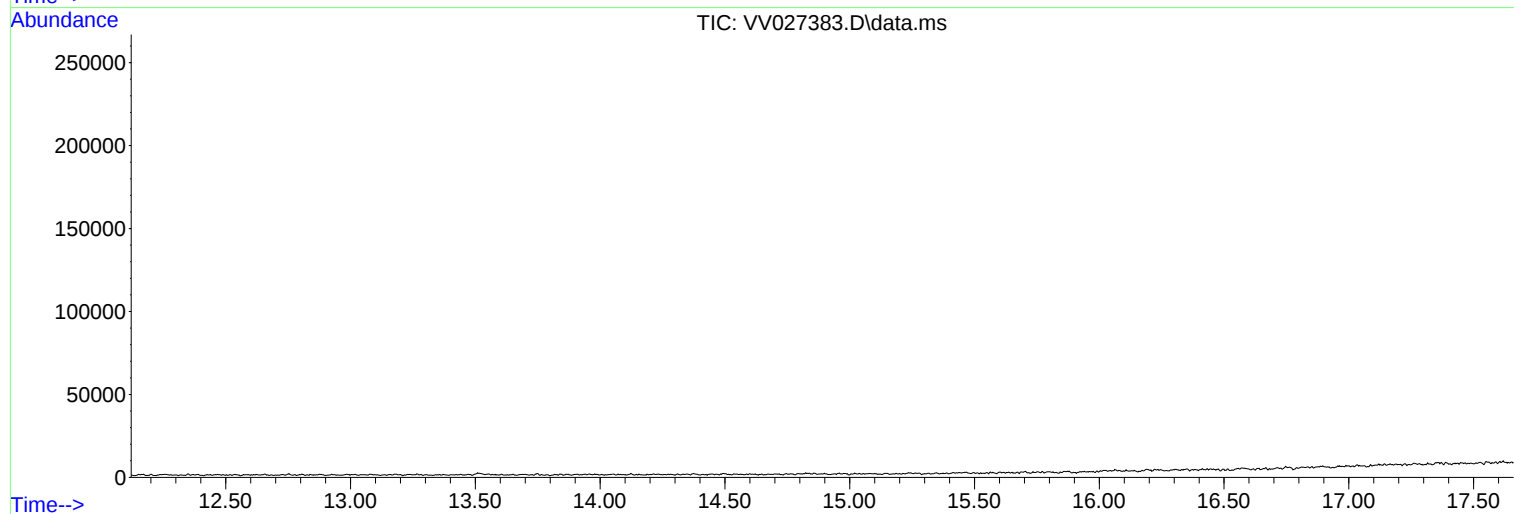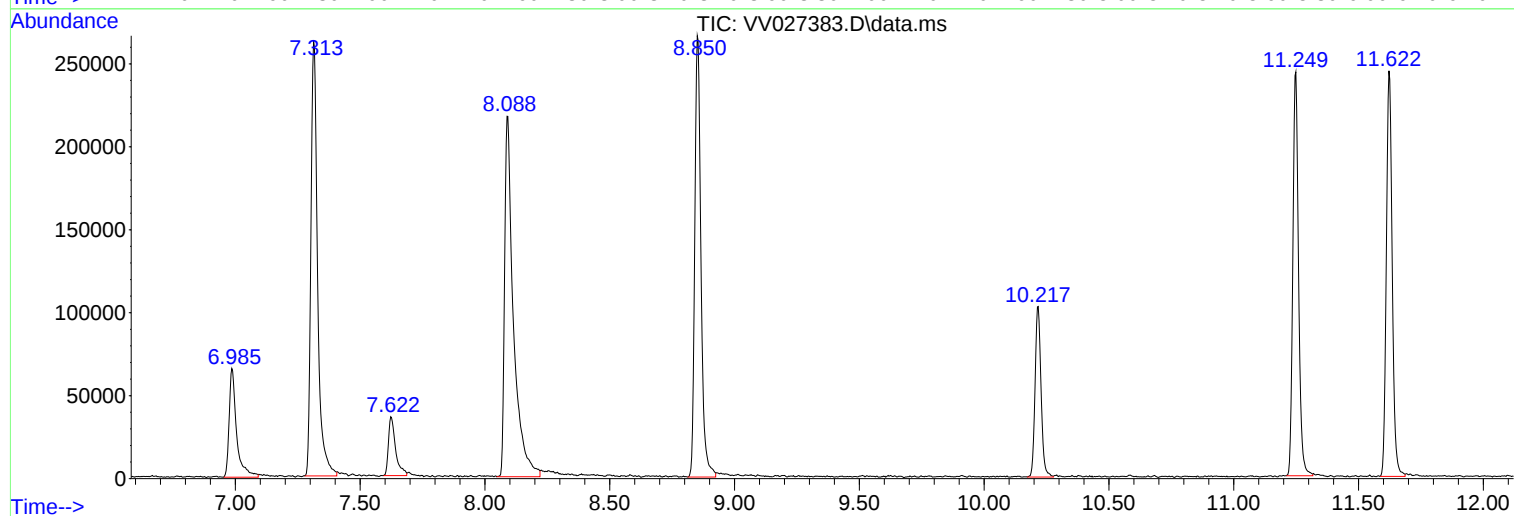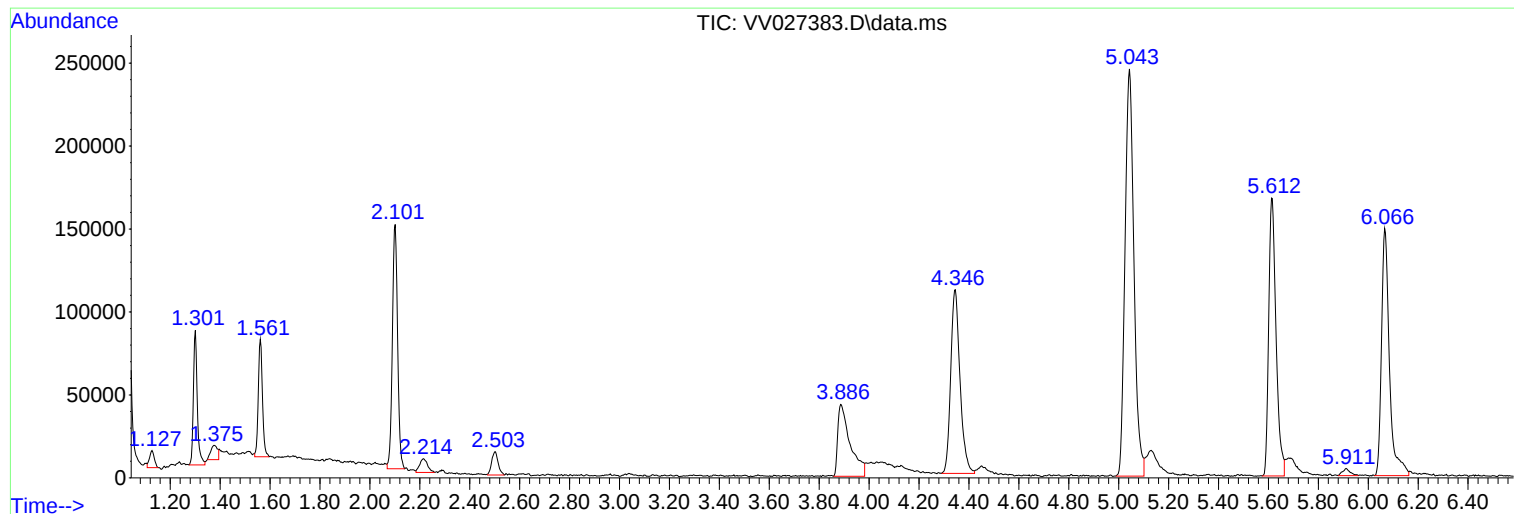

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027383.D
Acq On : 15 Aug 2022 12:30
Operator : SY/MD
Sample : N4162-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027383.D
Acq On : 15 Aug 2022 12:30
Operator : SY/MD
Sample : N4162-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc