

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027384.D
 Acq On : 15 Aug 2022 12:53
 Operator : SY/MD
 Sample : N4145-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027384.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	24	29	37	rVB2	11310	13510	2.25%	0.283%
2	1.304	75	82	95	rBV	74616	81234	13.56%	1.701%
3	1.388	100	108	110	rBV2	8411	11586	1.93%	0.243%
4	1.564	156	163	176	rVB	70245	82289	13.73%	1.723%
5	2.105	321	331	346	rVB	142455	208747	34.83%	4.371%
6	2.224	360	368	382	rVB	9212	16744	2.79%	0.351%
7	2.506	445	456	468	rVB2	13529	24121	4.03%	0.505%
8	3.889	877	886	908	rBV	40953	131275	21.91%	2.749%
9	4.346	1012	1028	1053	rBV2	105357	278987	46.56%	5.842%
10	5.043	1229	1245	1266	rBV2	238559	599263	100.00%	12.549%
11	5.616	1409	1423	1440	rBV	175851	363532	60.66%	7.613%
12	5.911	1500	1515	1521	rBV	4645	10070	1.68%	0.211%
13	6.069	1547	1564	1579	rBV	147039	304363	50.79%	6.374%
14	6.989	1839	1850	1875	rBV	59851	126633	21.13%	2.652%
15	7.313	1939	1951	1983	rBV	252310	476494	79.51%	9.978%
16	7.625	2033	2048	2064	rBV	35603	72652	12.12%	1.521%
17	8.091	2182	2193	2232	rBV	214641	528131	88.13%	11.059%
18	8.850	2418	2429	2457	rBV	277939	484113	80.78%	10.138%
19	10.214	2843	2853	2869	rBV	100173	166173	27.73%	3.480%
20	11.246	3163	3174	3199	rBV	247926	407020	67.92%	8.523%
21	11.622	3277	3291	3309	rBV	241319	388424	64.82%	8.134%




Sum of corrected areas: 4775361

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027384.D
Acq On : 15 Aug 2022 12:53
Operator : SY/MD
Sample : N4145-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

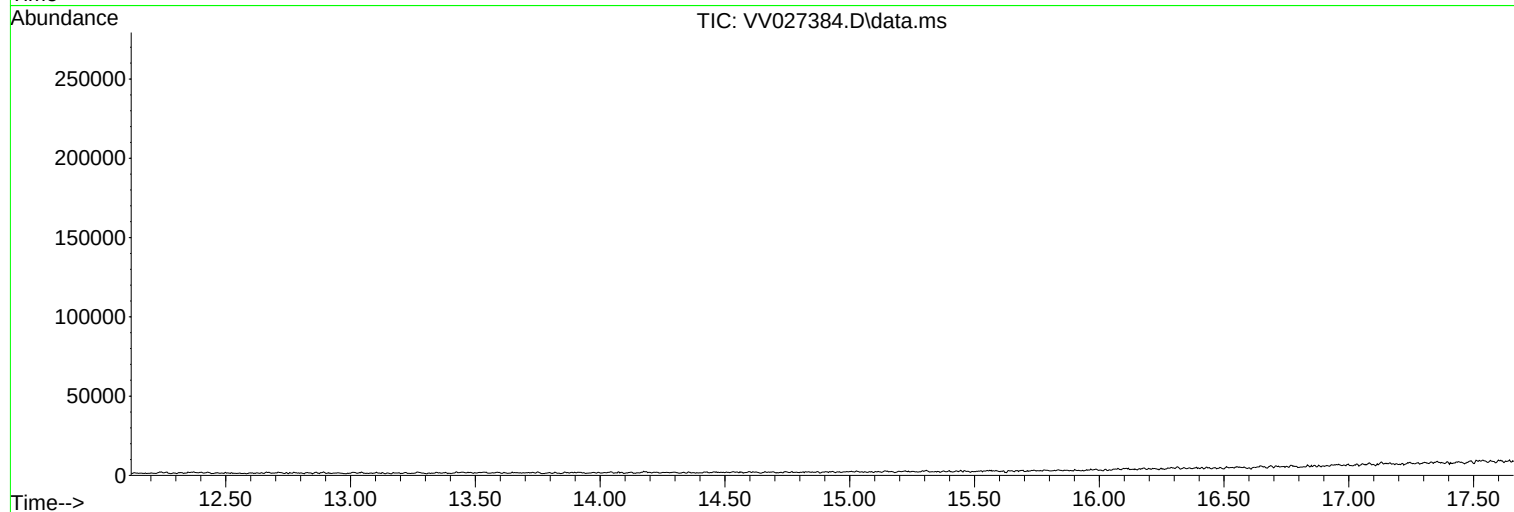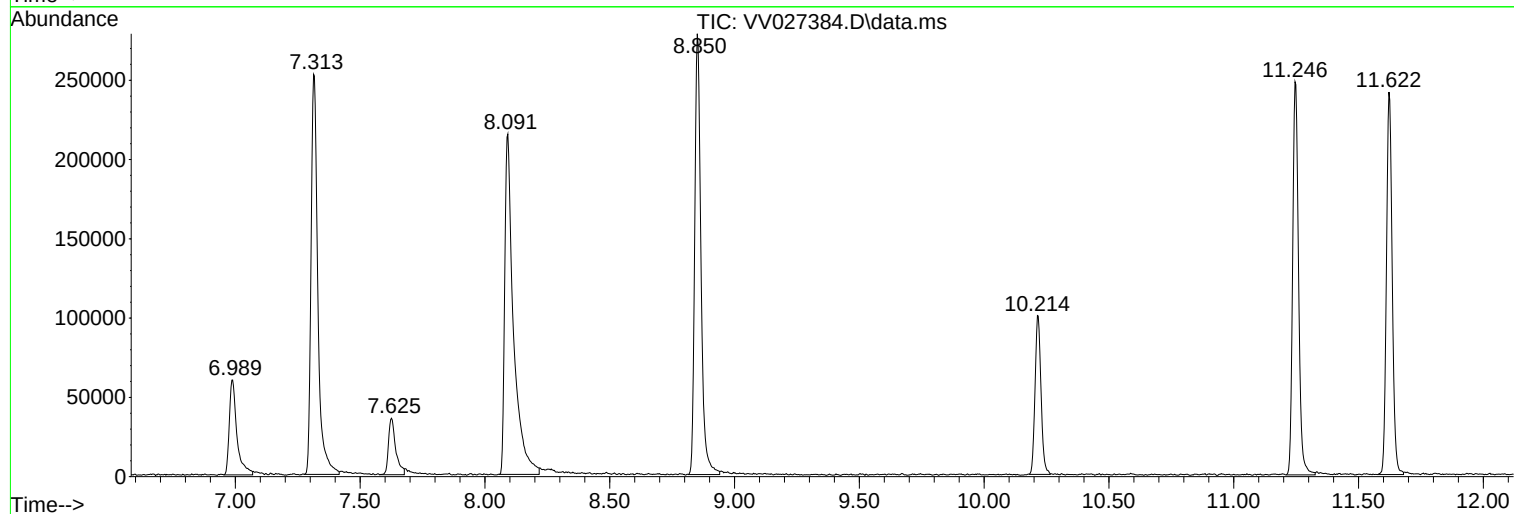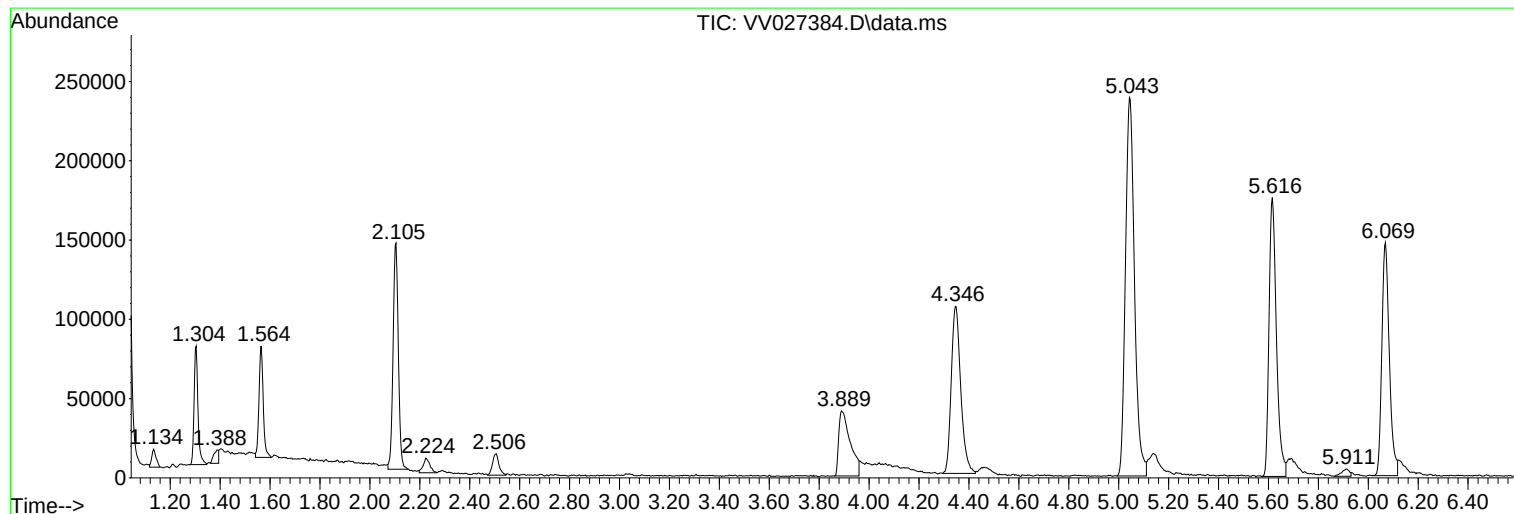

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027384.D
Acq On : 15 Aug 2022 12:53
Operator : SY/MD
Sample : N4145-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027384.D
Acq On : 15 Aug 2022 12:53
Operator : SY/MD
Sample : N4145-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc