

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027386.D
 Acq On : 15 Aug 2022 13:41
 Operator : SY/MD
 Sample : N4133-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027386.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.133	24	29	39	rVB2	9585	13198	2.22%	0.278%
2	1.301	75	81	99	rVB	75530	82708	13.91%	1.740%
3	1.394	99	110	112	rBV3	11259	20048	3.37%	0.422%
4	1.561	156	162	176	rVB	65374	78608	13.22%	1.654%
5	2.101	320	330	347	rVB	144424	212323	35.71%	4.467%
6	2.223	359	368	382	rVB4	8022	15252	2.56%	0.321%
7	2.503	444	455	467	rBV2	9666	16755	2.82%	0.352%
8	3.889	878	886	917	rBV	44443	159989	26.90%	3.366%
9	4.346	1012	1028	1052	rBV3	110959	284285	47.81%	5.981%
10	5.043	1229	1245	1266	rBV2	237005	594652	100.00%	12.510%
11	5.616	1410	1423	1442	rBV	172119	359266	60.42%	7.558%
12	6.069	1548	1564	1580	rBV	145480	310228	52.17%	6.526%
13	6.985	1839	1849	1868	rBV	59088	118215	19.88%	2.487%
14	7.313	1939	1951	1981	rBV	250636	468435	78.77%	9.855%
15	7.625	2037	2048	2073	rBV2	34248	70540	11.86%	1.484%
16	8.091	2183	2193	2223	rBV	221535	523455	88.03%	11.012%
17	8.850	2419	2429	2453	rBV	280254	474364	79.77%	9.979%
18	10.217	2841	2854	2869	rBV	103571	170803	28.72%	3.593%
19	11.249	3164	3175	3192	rBV	244685	393785	66.22%	8.284%
20	11.622	3275	3291	3310	rBV	245706	386487	64.99%	8.131%




Sum of corrected areas: 4753396

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027386.D
Acq On : 15 Aug 2022 13:41
Operator : SY/MD
Sample : N4133-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

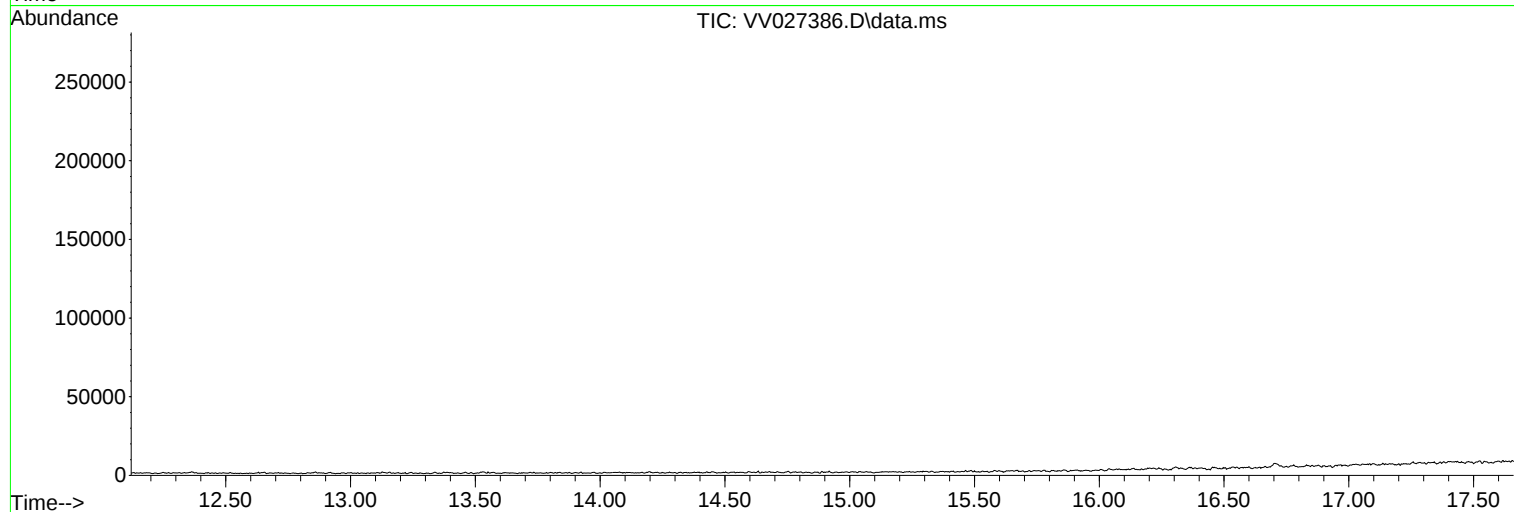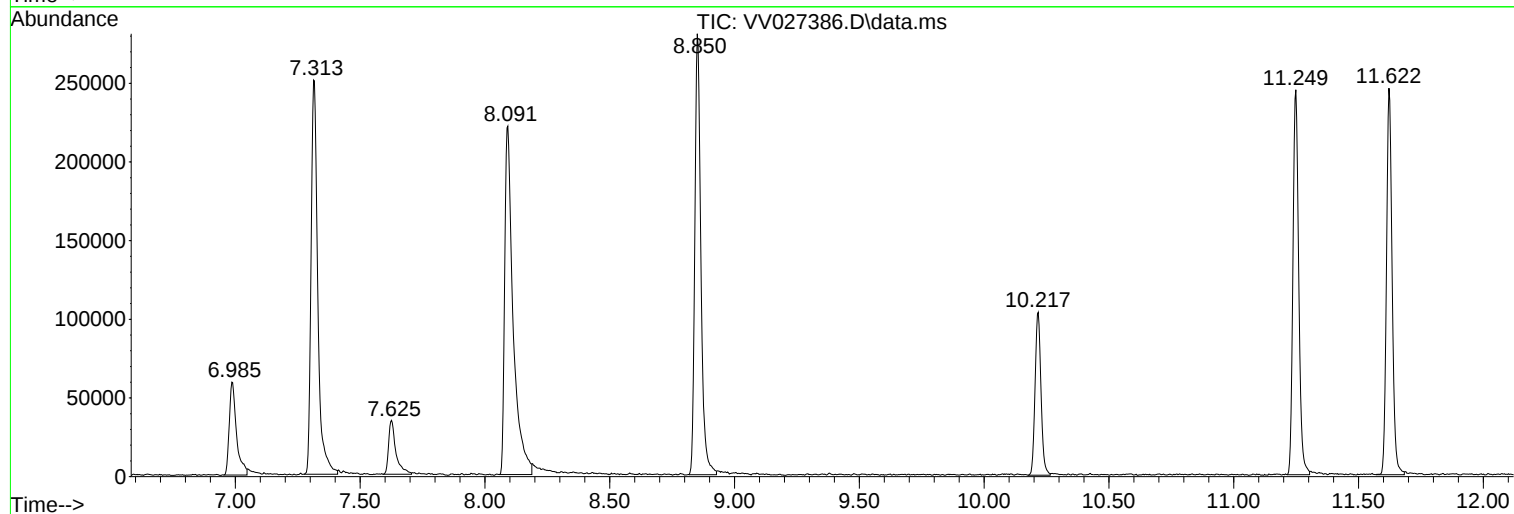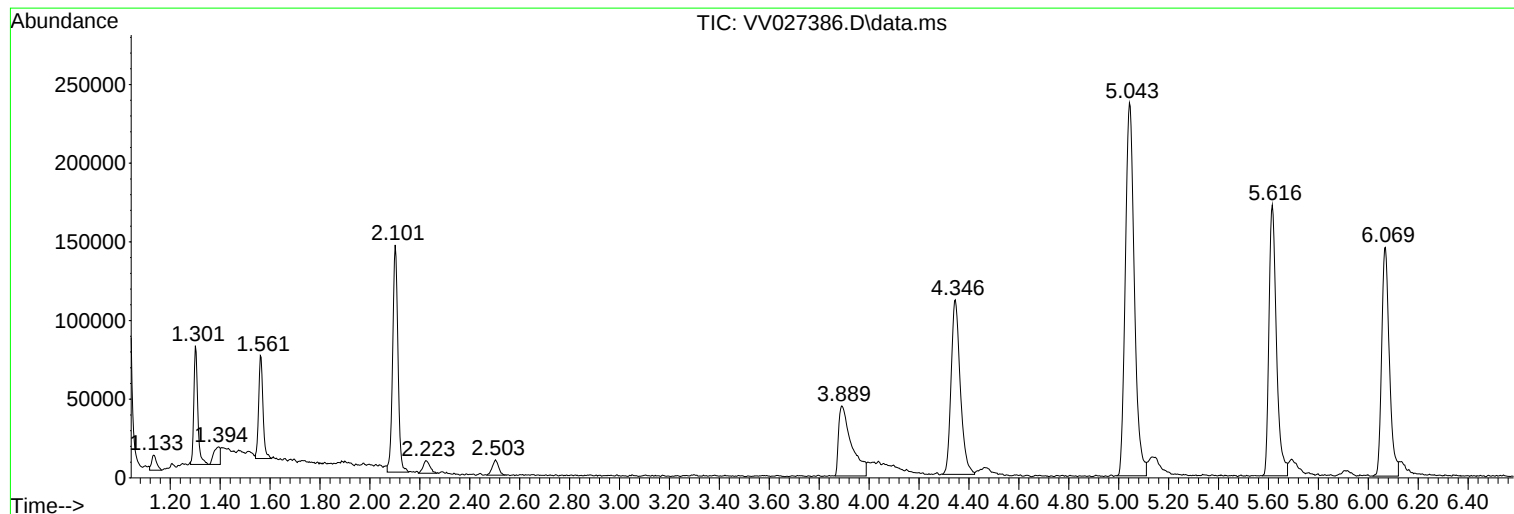

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027386.D
Acq On : 15 Aug 2022 13:41
Operator : SY/MD
Sample : N4133-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027386.D
Acq On : 15 Aug 2022 13:41
Operator : SY/MD
Sample : N4133-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
