

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027390.D
 Acq On : 15 Aug 2022 15:33
 Operator : SY/MD
 Sample : N4096-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027390.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.143	25	32	44	rVB2	6509	10186	1.83%	0.228%
2	1.301	74	81	95	rBV	70480	77036	13.85%	1.725%
3	1.384	100	107	109	rBV2	7540	9505	1.71%	0.213%
4	1.561	156	162	181	rVB	63756	78254	14.07%	1.752%
5	2.101	320	330	343	rVB	130729	192840	34.66%	4.317%
6	2.233	361	371	383	rVB2	8404	15298	2.75%	0.342%
7	2.503	444	455	461	rBV2	7286	12809	2.30%	0.287%
8	3.886	876	885	913	rBV	42529	140945	25.34%	3.155%
9	4.339	1008	1026	1055	rBV	102530	271753	48.85%	6.084%
10	5.040	1227	1244	1264	rBV2	222184	556311	100.00%	12.454%
11	5.612	1409	1422	1440	rBV	164766	343731	61.79%	7.695%
12	5.693	1445	1447	1458	rVB4	7821	11022	1.98%	0.247%
13	6.063	1547	1562	1578	rBV	135949	287275	51.64%	6.431%
14	6.985	1838	1849	1868	rBV	54427	109867	19.75%	2.460%
15	7.313	1939	1951	1977	rBV	229449	430253	77.34%	9.632%
16	7.622	2036	2047	2061	rBV2	32678	62053	11.15%	1.389%
17	8.088	2182	2192	2226	rBV	205784	495264	89.03%	11.087%
18	8.850	2413	2429	2453	rBV	262981	457459	82.23%	10.241%
19	10.214	2839	2853	2868	rBV	97743	161120	28.96%	3.607%
20	11.246	3163	3174	3194	rBV	238671	379489	68.22%	8.495%
21	11.622	3278	3291	3311	rBV	225468	364555	65.53%	8.161%




Sum of corrected areas: 4467025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027390.D
Acq On : 15 Aug 2022 15:33
Operator : SY/MD
Sample : N4096-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

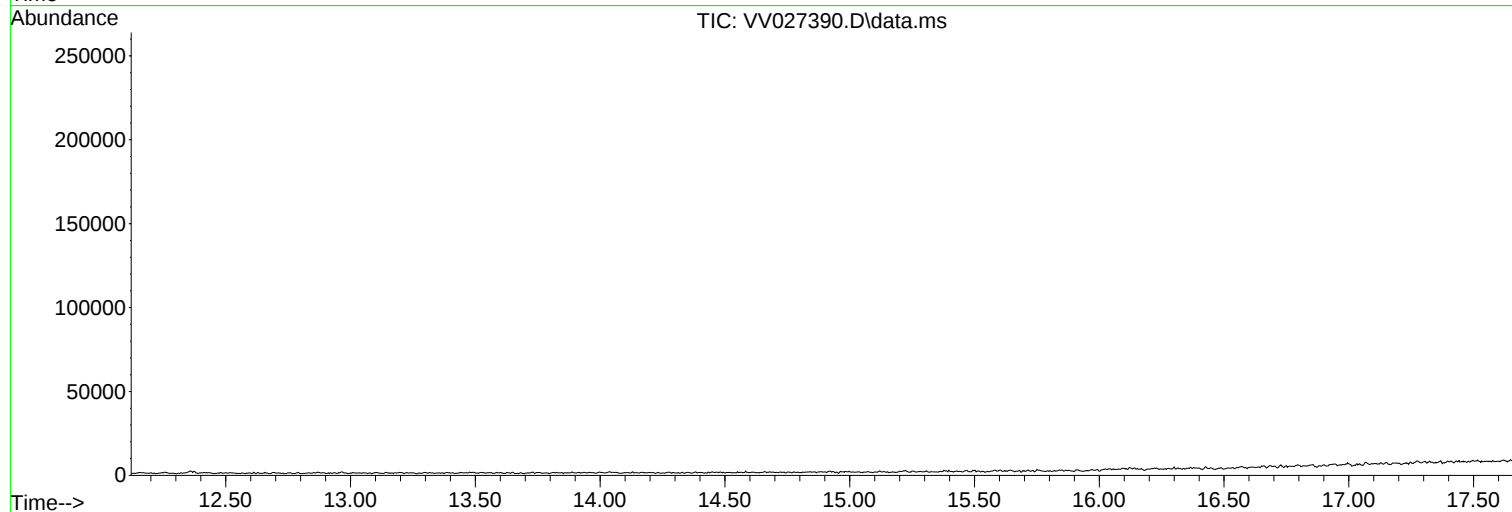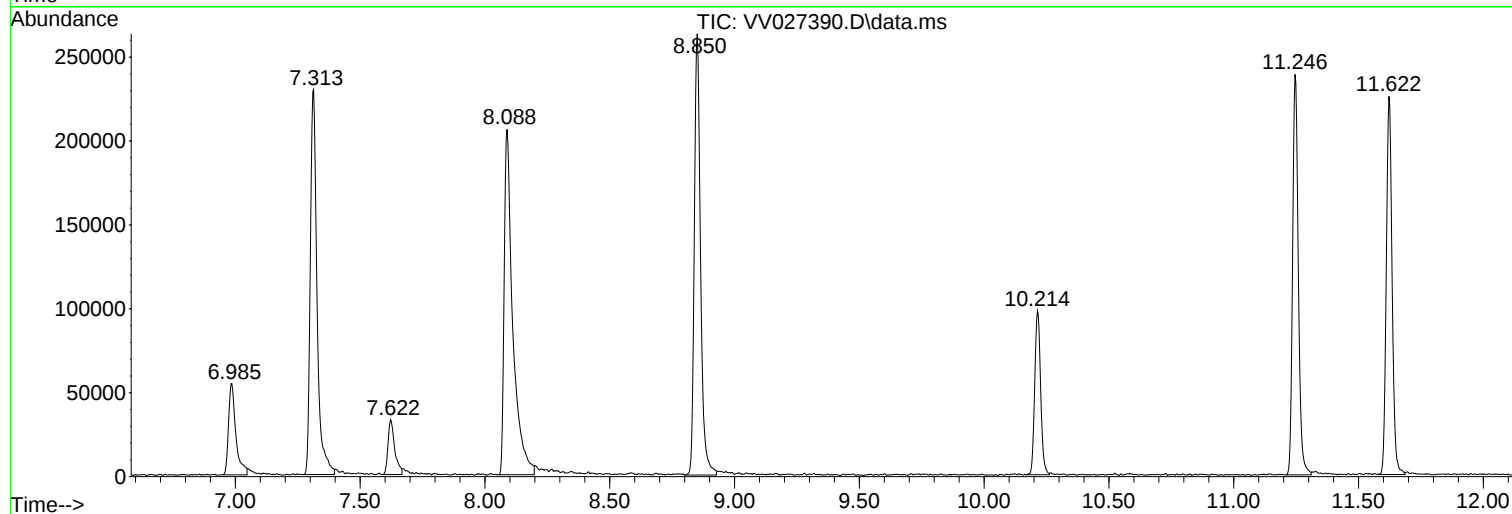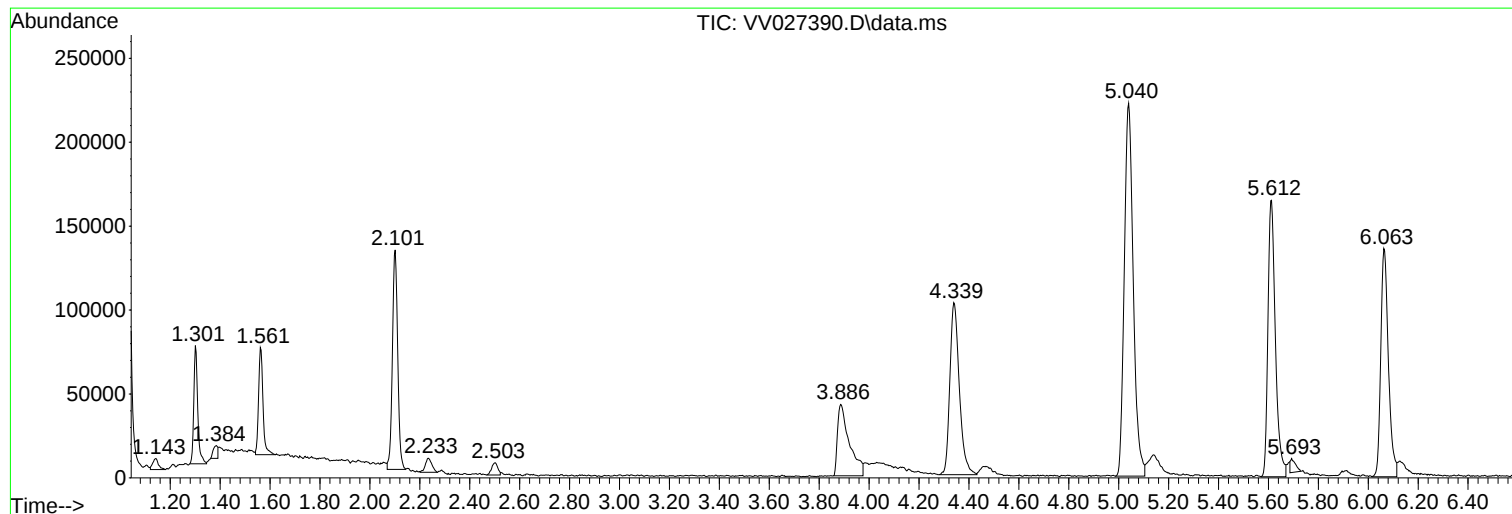

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027390.D
Acq On : 15 Aug 2022 15:33
Operator : SY/MD
Sample : N4096-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027390.D
Acq On : 15 Aug 2022 15:33
Operator : SY/MD
Sample : N4096-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc