

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027396.D
 Acq On : 15 Aug 2022 18:52
 Operator : SY/MD
 Sample : N4195-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CZ0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027396.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.236	56	61	72	rBV5	6638	12393	2.28%	0.270%
2	1.301	75	81	97	rVB	65356	68140	12.53%	1.486%
3	1.397	101	111	112	rBV8	10198	15724	2.89%	0.343%
4	1.561	156	162	172	rVB	56613	63605	11.69%	1.387%
5	2.101	321	330	343	rVB	114359	165279	30.39%	3.604%
6	2.172	345	352	361	rVB	6238	10125	1.86%	0.221%
7	2.259	370	379	389	rBV2	6782	12492	2.30%	0.272%
8	3.889	876	886	916	rBV2	56510	203019	37.33%	4.427%
9	4.342	1010	1027	1054	rBV	100480	262316	48.23%	5.720%
10	4.490	1068	1073	1084	rVB3	4126	6800	1.25%	0.148%
11	5.043	1228	1245	1269	rBV2	213288	543353	99.90%	11.849%
12	5.162	1272	1282	1294	rVB5	8828	20553	3.78%	0.448%
13	5.612	1410	1422	1444	rBV	171631	356862	65.61%	7.782%
14	6.066	1550	1563	1581	rBV	132667	280824	51.63%	6.124%
15	6.985	1835	1849	1865	rBV	54780	107487	19.76%	2.344%
16	7.313	1939	1951	1982	rBV	213434	407788	74.97%	8.893%
17	7.625	2036	2048	2065	rBV2	32144	66392	12.21%	1.448%
18	8.088	2181	2192	2226	rBV	250701	543908	100.00%	11.861%
19	8.850	2418	2429	2449	rBV	268766	459545	84.49%	10.021%
20	10.217	2840	2854	2866	rBV2	99950	160496	29.51%	3.500%
21	11.249	3163	3175	3192	rBV	243148	385125	70.81%	8.398%
22	11.532	3254	3263	3281	rBV4	20239	46074	8.47%	1.005%
23	11.622	3281	3291	3313	rVB	230620	369234	67.89%	8.052%
24	16.480	4795	4802	4812	rBV7	7018	12103	2.23%	0.264%
25	17.390	5079	5085	5090	rBV7	4529	6005	1.10%	0.131%




Sum of corrected areas: 4585642

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027396.D
Acq On : 15 Aug 2022 18:52
Operator : SY/MD
Sample : N4195-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

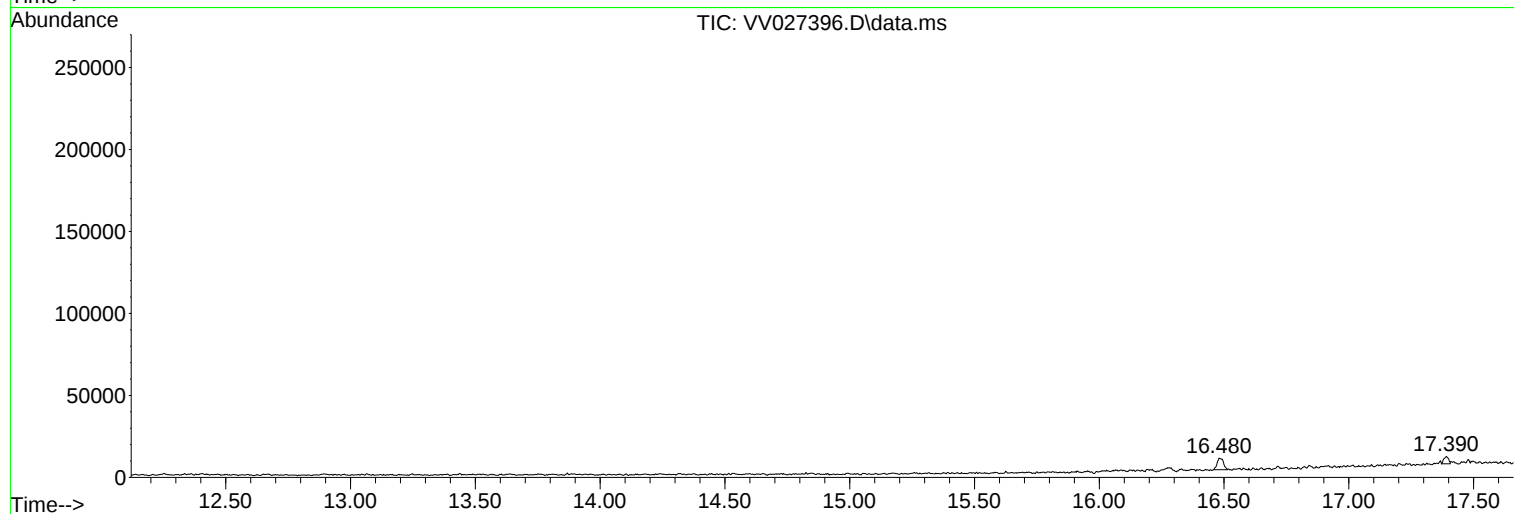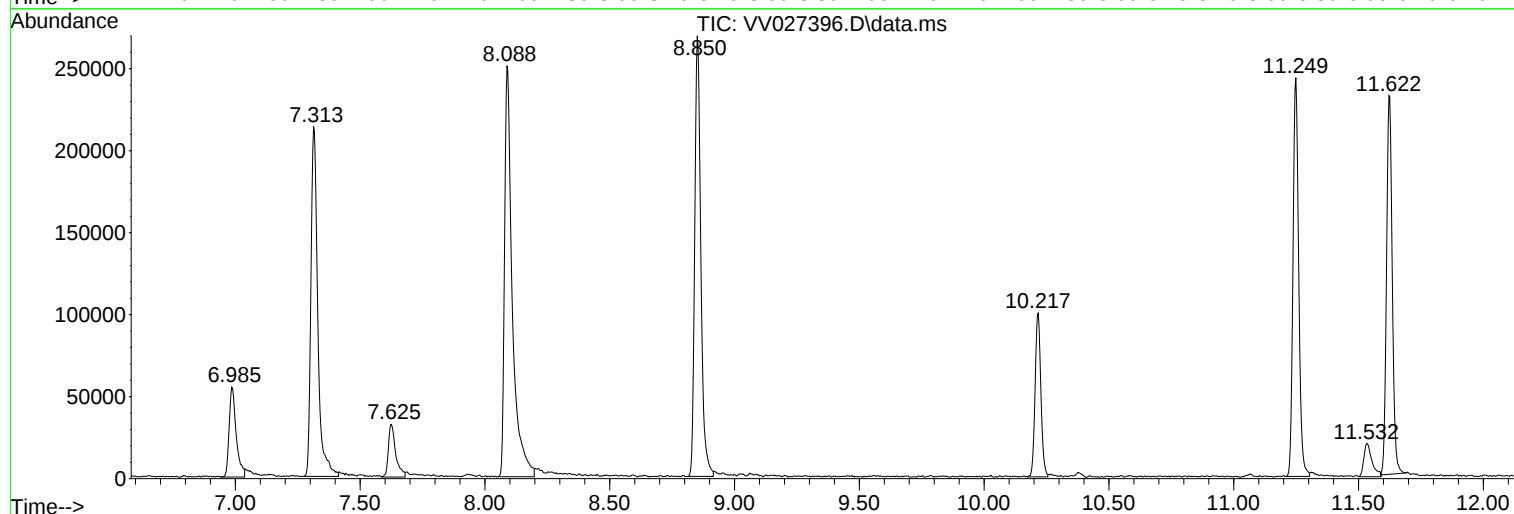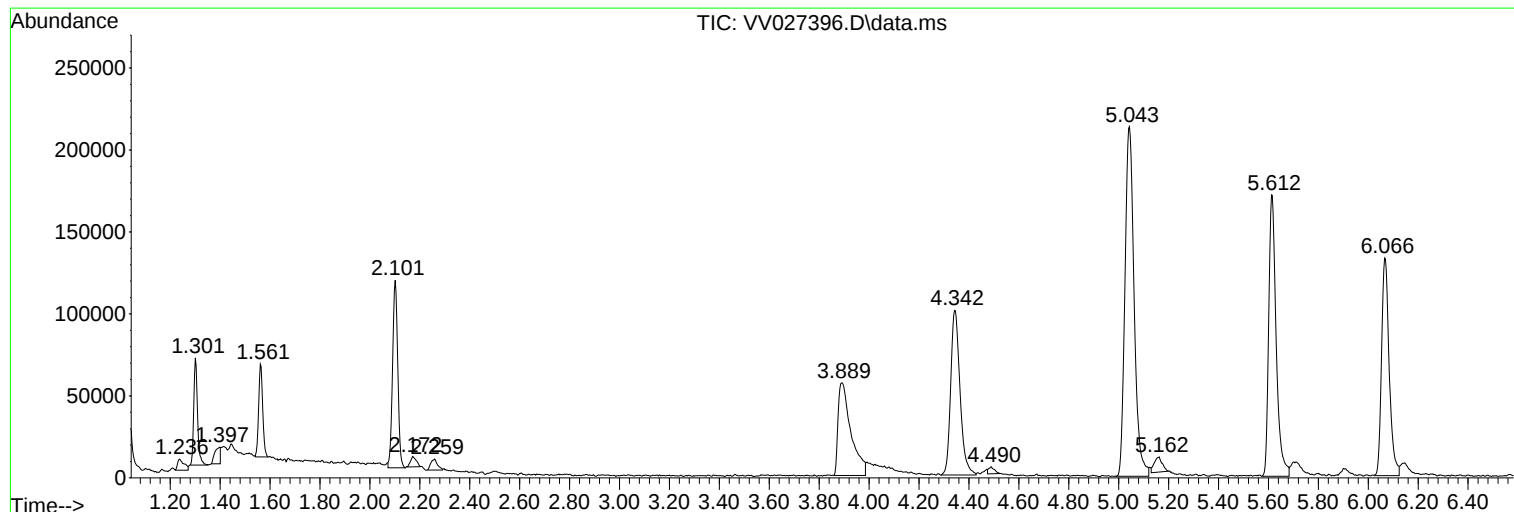

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027396.D
Acq On : 15 Aug 2022 18:52
Operator : SY/MD
Sample : N4195-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CZ0










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1-Hexanol, 2-ethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.532	0.60 ug/L	46074	1,4-Dichlorobenzene-d4	11.249

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	78
2	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	78
3	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	72
4	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	72
5	2-Propyl-1-pentanol			130	C8H18O	058175-57-8	53

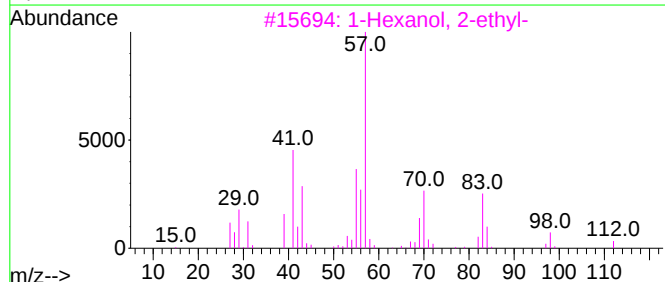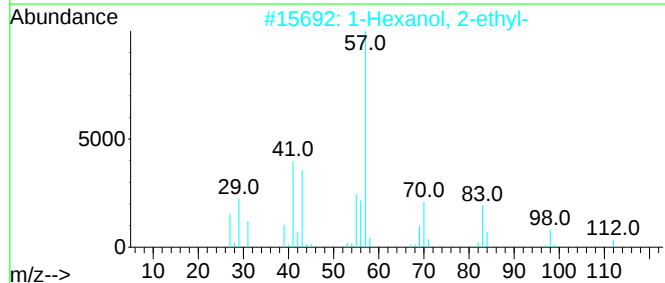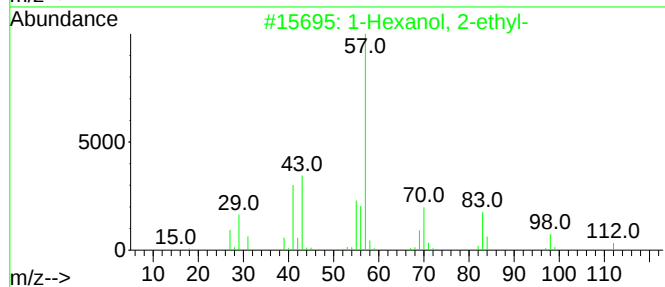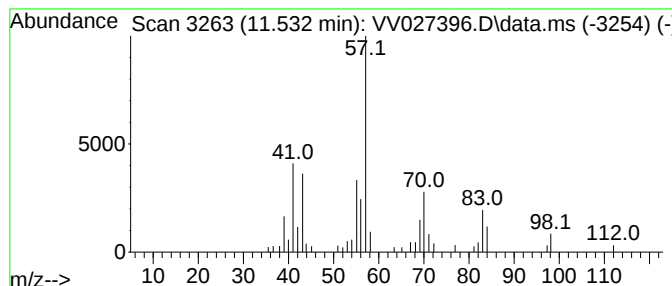

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027396.D
Acq On : 15 Aug 2022 18:52
Operator : SY/MD
Sample : N4195-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexanol, 2-et...	11.532	0.6	ug/L	46074	3	11.249	385125	5.0