

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027398.D
 Acq On : 15 Aug 2022 19:42
 Operator : SY/MD
 Sample : N4195-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027398.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.159	33	37	48	rVB	5367	6788	1.22%	0.150%
2	1.301	74	81	94	rBV	66404	73587	13.24%	1.627%
3	1.564	156	163	177	rVB	61496	70496	12.69%	1.559%
4	2.101	321	330	351	rVB	122357	179975	32.39%	3.980%
5	2.249	364	376	389	rBV3	8586	16371	2.95%	0.362%
6	2.500	446	454	465	rBV	9125	15048	2.71%	0.333%
7	3.889	876	886	908	rBV2	43130	137866	24.81%	3.049%
8	4.346	1014	1028	1054	rBB2	96781	256282	46.12%	5.668%
9	5.043	1227	1245	1269	rBV3	217353	555668	100.00%	12.289%
10	5.146	1273	1277	1290	rVB4	8608	17480	3.15%	0.387%
11	5.616	1411	1423	1441	rBV	169190	352499	63.44%	7.796%
12	5.699	1444	1449	1474	rVB3	9881	26355	4.74%	0.583%
13	6.066	1550	1563	1580	rBV	135987	286416	51.54%	6.335%
14	6.985	1837	1849	1879	rBV	54519	114077	20.53%	2.523%
15	7.313	1938	1951	1986	rBV	222622	421854	75.92%	9.330%
16	7.625	2038	2048	2069	rBV2	33007	66497	11.97%	1.471%
17	8.091	2181	2193	2229	rBV	213947	536089	96.48%	11.856%
18	8.850	2418	2429	2456	rBV	271799	463889	83.48%	10.260%
19	10.217	2843	2854	2869	rBV	101466	165453	29.78%	3.659%
20	11.249	3163	3175	3196	rBV	246958	391994	70.54%	8.670%
21	11.622	3278	3291	3313	rVV	228619	366803	66.01%	8.112%




Sum of corrected areas: 4521487

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027398.D
Acq On : 15 Aug 2022 19:42
Operator : SY/MD
Sample : N4195-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

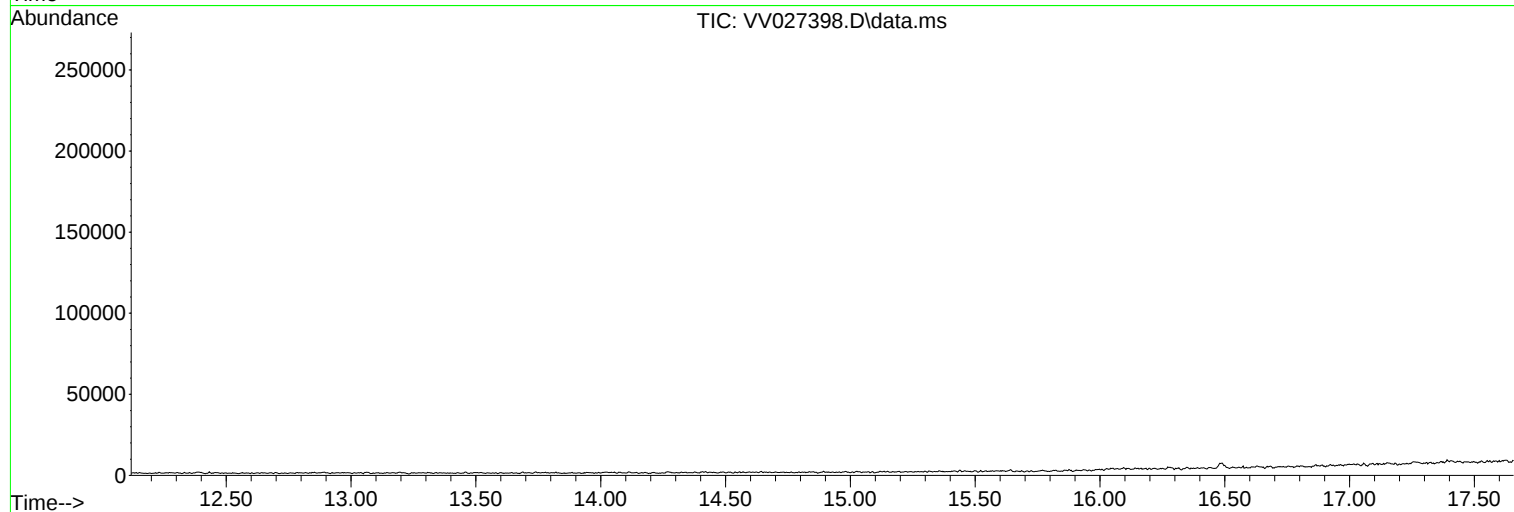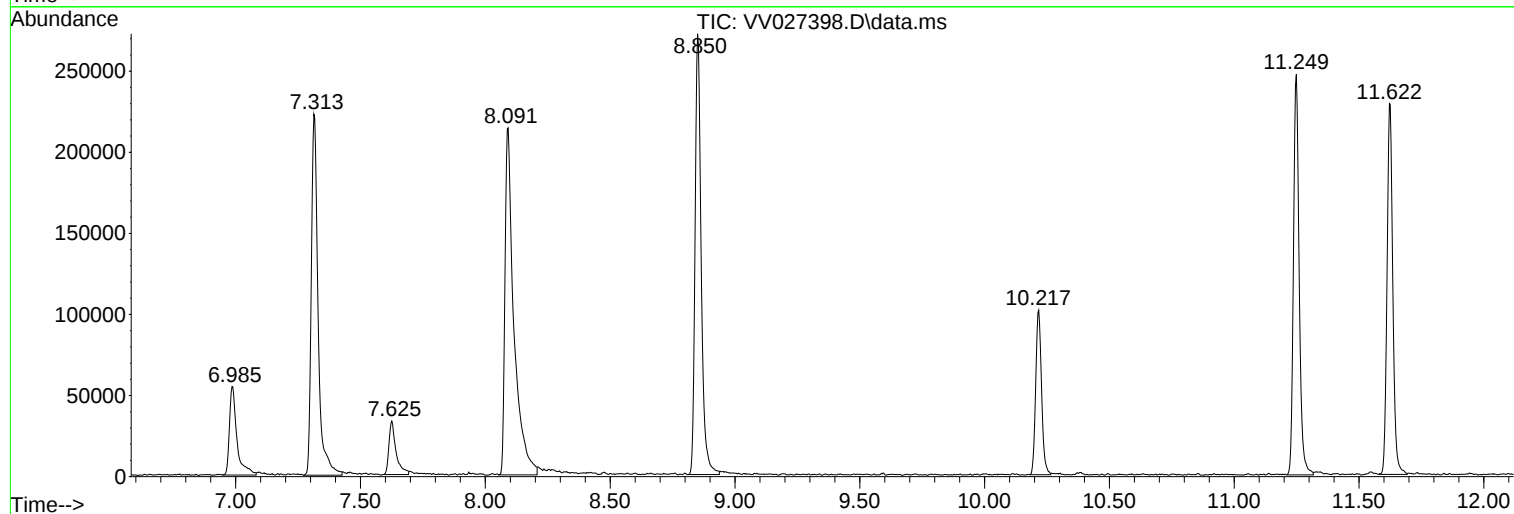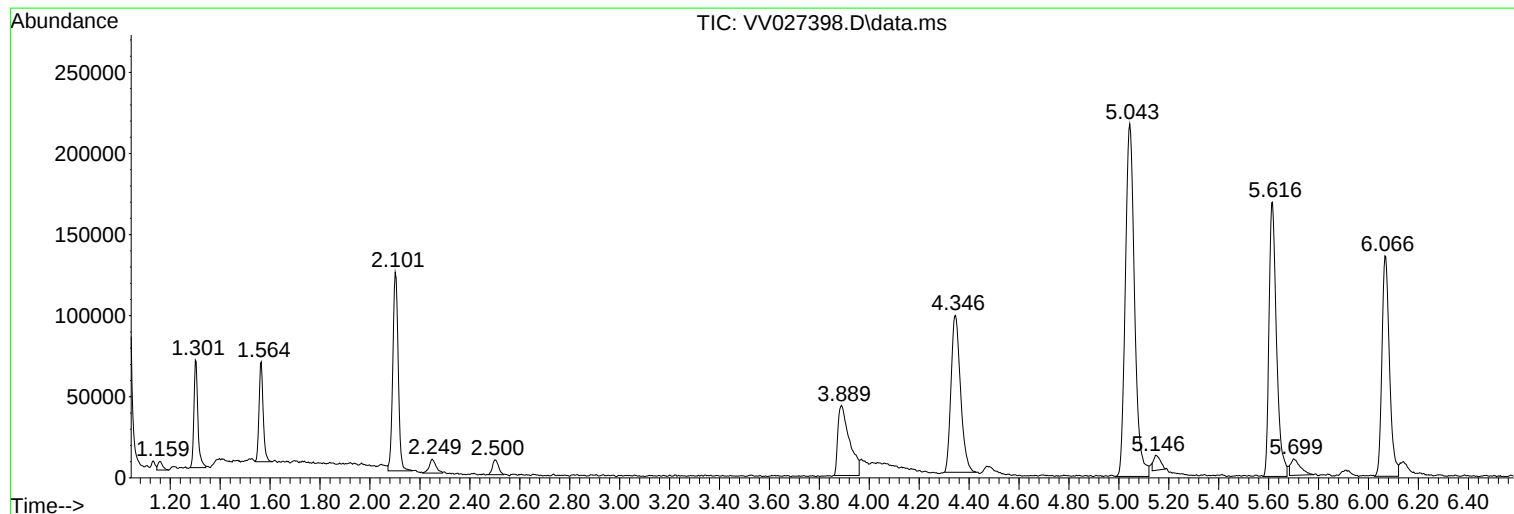

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027398.D
Acq On : 15 Aug 2022 19:42
Operator : SY/MD
Sample : N4195-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
Data File : VV027398.D
Acq On : 15 Aug 2022 19:42
Operator : SY/MD
Sample : N4195-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
